







Wahsita



YouTube



Youtube-EDA Channel



Facebook



ΦΛΩΡΟΣ DENTAL plus

Εγνατία 88, 54623 Θεσσαλονίκη, Τηλ. 2310 224203

www.florosdental.gr - info@florosdental.gr



Changzhou Sifary Medical Technology Co., Ltd

Add: NO.99, Qingyang Road, Xuejia County, Xinbei District, Changzhou City, 213000 Jiangsu, China Email: ivy@sifary.com Web: www.eighteeth.com





### CATALOG

1	Di Impress	gital ions	3	Imaging Sys	stems
	Helios 600 Intraoral Scanner	01-06		HyperLight  Portable X-ray unit  HyperLight-G	43-46 47-48
2	Handpiec Small Equipn			Portable X-ray unit  NanoPix Intraoral X-Ray Sensor	49-52
	E-xtreme Make Essence to Extreme	07-08	4		ptics
	E-connect Cordless Endo Motor	09-10			
	E-value Brushless Endo Motor	11-12		Brilliance Dental Loupes	53-54
	E-connect S Endomotor With Built-in Apex Locator	13-14		Softouch Surgical Headlight	55-56
	Ultra X Cordless Ultrasonic Activator	15-16			
	UltraMint & UltraMint Pro All-round Ultrasonic Scaler	17-22	5	Mat	erials
	CuringPen 4 LEDs curing light	23-24			
	CuringPen-E 3 LEDs Curing Light	25-26		UltraClean Antibacterial Root Canal Cleanser	57-58
	Fast-Pack pro & Fast-Fill Cordless Obturationgs System	27-34		E-FLEX Series NiTi Endo File	59-78
	E-PEX Apex Locator	35-36			
	AirPex Wireless Apex Locator	37-38			
	Motorturbo & E-Asp 1 Electric Motor and 1:5 handpiece	39-42			







### Start your smooth digital journey with Helios 600!

### Why bother?

High accuracy with automatic and adaptive calibration, manual calibration is not necessary any more.

### Ready for your digital experience-

One of the most accurate and fastest scanners on the market.

### Ready for your hand-

Small enough to operate it easily, though it achieves a 16mm x 14mm high-definition field of view.





198 grams, one of the most lightweight scanners on the market, well-balanced, ergonomically designed, and easy to carry.



With Helios 600 you can take a full arch scan in less than 30 seconds.




### Smarter

Al technology filters the soft and moving tissues, offering users a smooth scanning experience and generating a natural-looking treatment outcomes.



### More accurate

As one of the most accurate scanners on the market, Helios 600 has reached the state-of-the-art accuracy level- the average deviation of a in-vivo full arch scan is around 20µm.

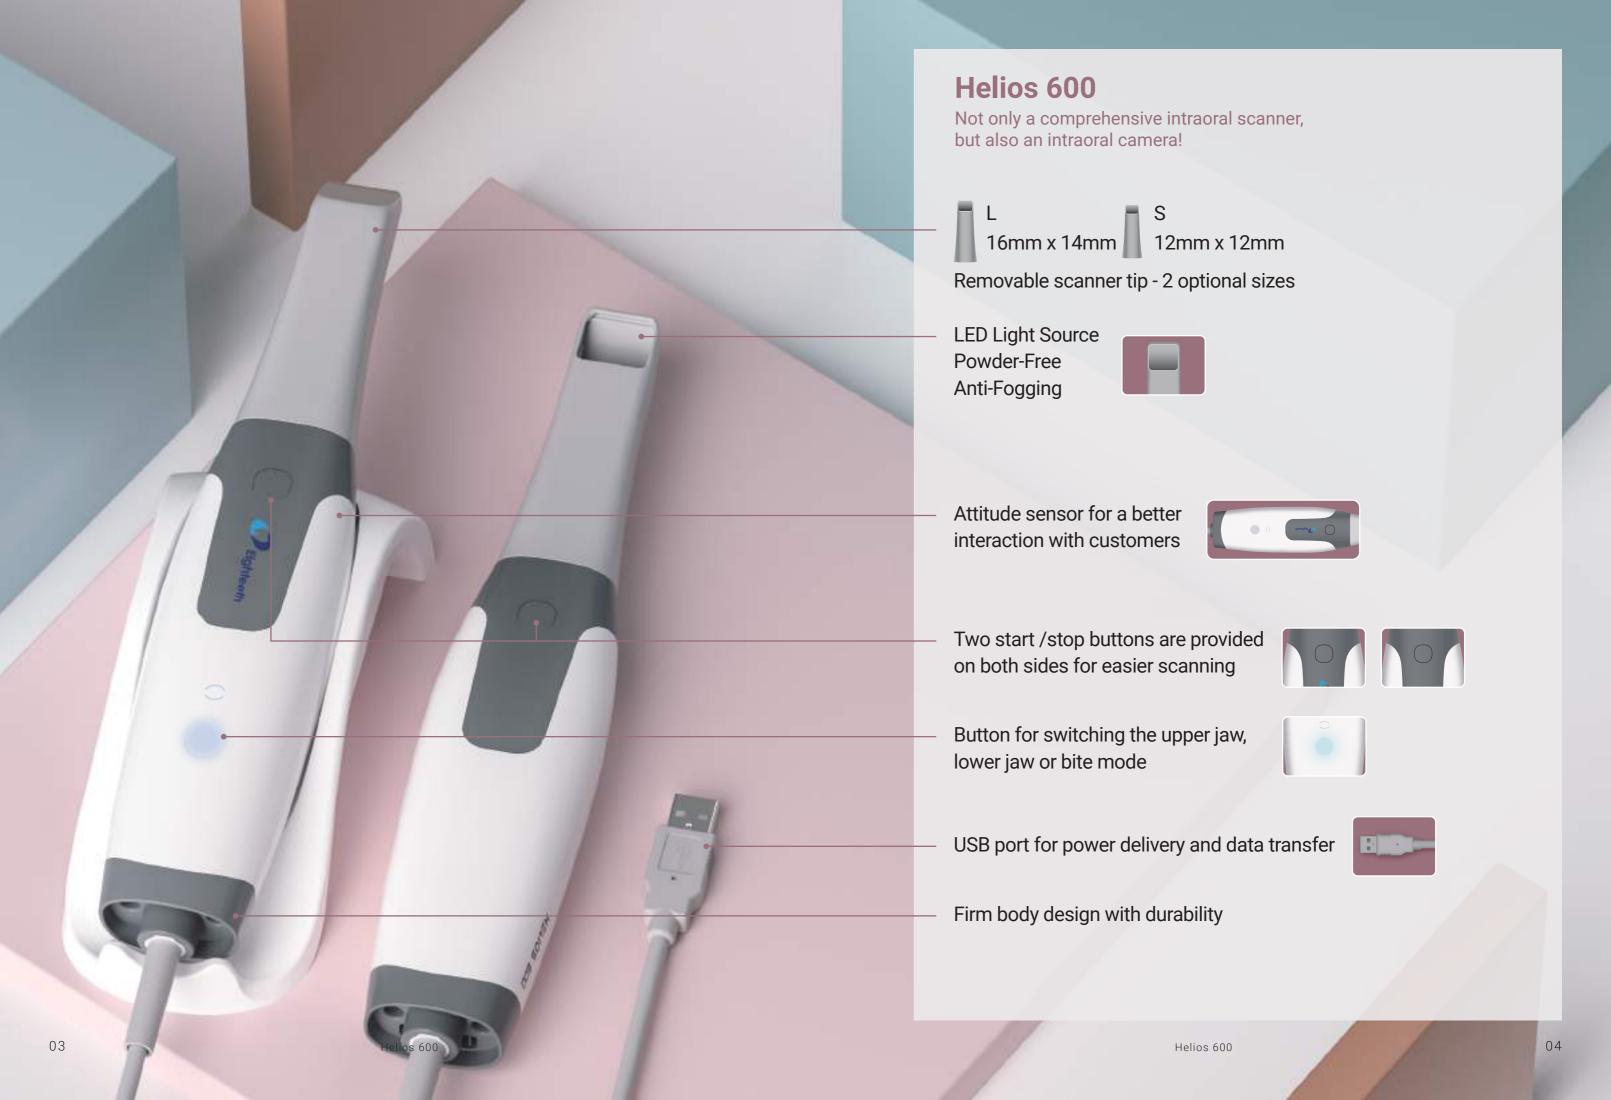





### Plug & Scan



Smart Reminder



Air mouse



Automatic software update



Timely after-sales service



Cloud Storage



Voice Memo



Online 3D viewer

### **Specification**

### Helios 600

Accuracy	Full-arch 20.0µm		
0	16 x 14mm (L)		
Scan area	12 x 12mm (S)		
	Dimension	219 x 46 x 36mm	
Handpiece	Weight	198g	
	Capture button	Two sided	
Tip	Tip size (front part)	22 x 18mm (L)	
Tip		18.6 x 16.7mm (S)	
Connectivity	Length	1.8m	
Connectivity	Туре	USB 3.0	
Calibration	Accuracy calibration	Calibration-free	
Calibration	Color calibration Calibration-free		
Special mode	Remote control mode		

### Recommended System Requirements

Processor	Intel®CoreTM i7 9th Generation, base frequency 2.6 GHz (or better)	
Memory	16GB (or more) DDR4, frequency 2666 MHz (or better)	
Hard Drive	512GB (or more) SSD	
Graphics card	NVIDIA®GeForce®GTX 1650 (or better)	
Display	15.6" FHD (1920 x 1080) (or more)	
Others	USB 3.0 port	
Operating system	Windows 10 Pro	
Optional	Touch screen	

Helios 600 06



### E-xtreme

Make Essence to Extreme







360° contra-angle rotation



Slim and compact design for maximum comfort and mobility



Miniature contra-angle for better visibility & easier pos t erior access

Miniature contra-angle Super Mini head & thin neck



- Normal head & neck





Eighteeth innovative motor, cutting down the noise from inside, allowing you to experience the tranquility.



Less than 100 grams, reducing hand fatigue during treatment, providing the ultimate E-xtreme experience.





Reciprocation function







Built-in file system

### **Specifications**

Model : E-xtreme Power supply : 100 V-240 V Weight(grams) :99 g Frequency : 50 Hz / 60 Hz Torque range : 0.5 N.cm-4.0 N.cm Output : DC 5 V/1 A

07 08 E-xtreme E-xtreme







Low Noise Motor



Powerful 1500 mAh Lithium Battery



Integration Option



Screen Cast / Mirroring



Ambidextrous \* Display

\*User can rotate the Endomotor Screen towards left or right \*In connect function Endomotor mirrors Apex Locator's screen

### **Integrate Endomotor with Apex Locator** (Connect Function)



Auto Start & Stop



Apical Reverse



Apical Slow Down



### **Five Reciprocation Modes (M0)**



Reverse Reciprocation-One Mode Counter clockwise & clockwise movement

Fwd 30° - Rev 150° For reciprocating files



Forward Reciprocation-Four Modes Clockwise & counter clockwise movement

Fwd 150° - Rev 30° Fwd 180° - Rev 30° Fwd 210° - Rev 30° Fwd 250° - Rev 30° For all continuous rotation files



### Nine Editable Memory Programs (M1 to M9)



Editable Torque setting



Forward Direction of Rotation



360° Clockwise Rotational Movement



Reverse Direction of Rotation



Editable Speed / Rpm Setting



Torque Auto Reverse



### **One Piece Contra Angle Head**



360° Adjustable Handpiece



Detachable Head



Miniature Head



Autoclavable






### E-value

### **Brushless Endo Motor**

(1) Sighteeth



Speed Range : 120-1000 rpm

Torque Range : R.L-4.0 N.cm

Memory Programs : 10 (M1 to M10)





**OLED Color Screen**More comfortable visual experience



**Built-in File System**Switch file systems quickly



**360° Rotatable** 360° Rotatable Contra Angle



**Brushless Motor** Reliable, Durable, Efficient



Long Battery Life
Heavy capacity
1900mAh lithium battery



Mini Contra Angle Advanced 1:1 contra-angle One piece design





New contra-angle head

### **Built-in File System**



**Built-in File System** 

Long Press S to enter the Mode Setting interface

• • • Choose the Endo File

being used and press S

300rpm


3.0N cm

E-FLEX BLUE

MI

Fwd

Note: the doctor could adjust the speed, torque limit and reciprocating angle according to the needs of the case.

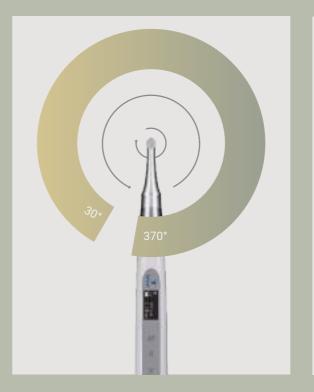

### **Working Modes:**

• Fwd- Forward Rotation

• Rev - Reverse Rotation

REC- Reciprocation Mode

Doctor could set the reciprocating angle and speed level according to actual needs

- -Speed Level range from Level 1 to Level 5
- -Angles range from 30° to 370°
- ATC- Adaptive Torque Control Mode

After reaching the preset torque limit, motor will reciprocate according to the set angle to improve the efficiency of root canal enlargement







E-value E-value 12



### E-connect S

Endomotor With Built-in Apex Locator





### **Torque Calibration**For precise torque output



**OLED Screen**Digital OLED Display



### **Ambidextrous Display**

Screen can be rotated as per Left or right hand use




### **Powerful Battery**

Heavy duty 1500mAh Lithium battery





Apex Locator Bar



### APEX LOCATOR

- Apical control with rotary instruments

  Position of file is displayed on screen and the motor rotates in reverse direction when file reaches pre-set apical working length, to prevent over instrumentation
- Manual canal measurement
   Manual file clip can be used to measure canals precisely with hand files
- Multi frequency technology with high accuracy & precision
- Apex locator flash bar with zoom-in function

### **Working Modes:**

FWD - Clockwise Continuous Rotation

**REV - Anti-clockwise Continuous Rotation** 

### **REC** - Reciprocation Movement

First-in-class cordless open motor with adjustable angles of rotation ranging from  $30^{\circ}$  to  $370^{\circ}$  for reciprocation as per user's need

First-in-class feature of speed adjustment in reciprocation mode

### **ATC** - Adaptive Torque Control

ATC manages the file stress in a smart way. When torque limit is reached, instead of going into reverse mode, motor reciprocates till the stress is reduced. Once back to below pre-set torque level, file will again rotate in continuous rotation

### **Integrated mode features:**

- Auto Start & Stop Motor starts working when the file enters inside root canal, and stops when withdrawn
- Apical Reverse When the file reaches pre-set apical reverse point, user can define whether the file starts moving in reverse direction
- Apical Slow Down To preserve the cemento-dentinal junction and avoid file separation, speed of motor slows down when file is in apical region

### **Specifications:**

Rotational Speed Range : 120-1000 rpm
Torque Range : 0.5-4.0 N.cm
Memory Programs : 11 (M0 to M10)
Battery Capacity : 1500 mAh

E-connect S E-connect S

27 Eighte eth



**Activator** 

### Available Tips

	•
Size	Length(mm)
#20 2%	18 & 21
#25 2%	18 & 21

Autoclavable

Tips





Smooth Surface Finish



Flexible Tips \*Only X Blue &



 $\chi$  Silver

Multiple Tip **Options** 




### In Action

### **Cavitation Effect**

It is the process of formation of millions of gas bubbles in the irrigation solution. These gas bubbles grow in size, oscillate in different directions and explode into the liquid, producing powerful cleaning action

### **Acoustic Streaming**

It is a unidirectional flow of liquid produced by ultrasonic waves. Movement of tip produces special effect called acoustic turbulence which accelerates the movement in liquid inside the root canal




### Indication

### Smear Layer Removal

Effective in removal of smear layer and unplugging of dentinal tubules

### **Dentin Chips Removal**

Ultrasonic agitation forms suspension of residual dentinal chips and tissue remnants with irrigant and facilitates their easy removal



### Indication

### **Biofilm Disruption**

Ultrasonic cavitation disrupts the biofilm and helps to reduce bacteria load in the canal

### Cleaning of Complex Anatomy

Ultrasonic activation helps irrigants to flush into undetected or un-instrumented canal anatomy like isthmus, fins, lateral canals, apical ramification etc. Also helps to remove vapour lock



### Protocol

- Prepare the root canal up to required size with the help of shaping and finishing instruments
- Choose the desired disinfectant and flushing agents for cleaning, debridement and disinfection of canals

  Fill the chosen irriation solution into the canal, never run Ultra X without irrigating solution
- Select the Ultra X tip of desired size and length which passively fits into canal, always keep 2 3mm short of apex Activate solution using short vertical up & down strokes for 30 seconds. Be careful to not breach apical 2mm
- Use the device gently and never apply pressure or wedge the tip inside the canal. If any points of resistance, then
- Replenish the irrigating solution, use suction to remove the loose debris. Repeat the cycle 4 to 5 times

Cordless

Irrigation Device

- Completely dry the canal and fll it with choice of obturation material
- It is always recommended to isolate the tooth using rubber dam and use personal protective barriers like head gear, mask, eyeglasses etc



1500 mAh

Powerful Battery

Application Based

Multiple Tips



Light Weight &

Ergonomic





### UltraMint & UltraMint Pro



### **Soft Perio Power for Ultimate Comfort**

Autoclavable plastic box - tips\*6, universal wrench\*1, EMS type handpiece\*1



Autoclavable plastic boxtips\*6, universal wrench\*1, Satelec type handpiece\*1 \*Applicable for all tips from Eighteeth

Smart touch system-ultrasensitive & waterproof



Intelligent self-cleaning-makes disinfection easy and avoids cross-infection



Two ways of water supply-Changing supply methods is easier than ever before



900ml stand-alone bottle with clear 20ml scale mark makes it convenient for formulating liquid.




Detachable handpiece with LEDautoclavable, ergonomic, brighter visibility





Detachable and autoclavable handpiece holder, resists cross-infection




Water control directly from handpiece



Ergonomic foot pedal




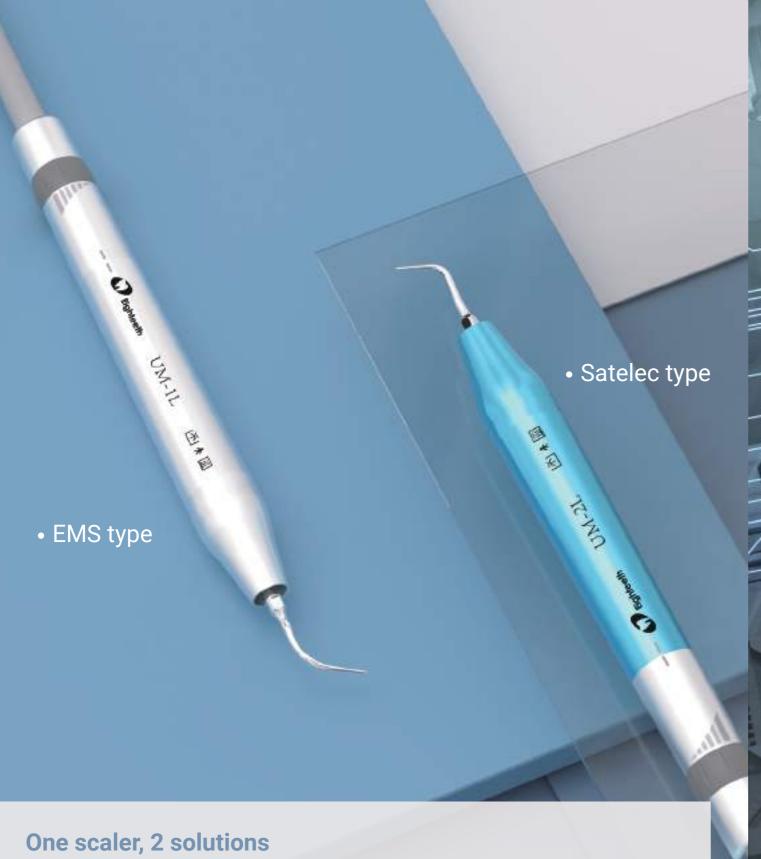

### Wide range of frequency: 25kHz-42kHz

 We are proud to give you two solutions to perform at your bestboth handpieces (EMS type and Satelec type) provided by Eighteeth are compatiable with UltraMint & UltraMint Pro.\* Scaling can be as convenient as you can imagine.

\*Satelec and EMS are trademarks of Acteor  $\!\!\!\!\!\!^{\mathrm{P}}$  and EMS  $\!\!\!\!\!\!^{\mathrm{P}}$  , respectively.

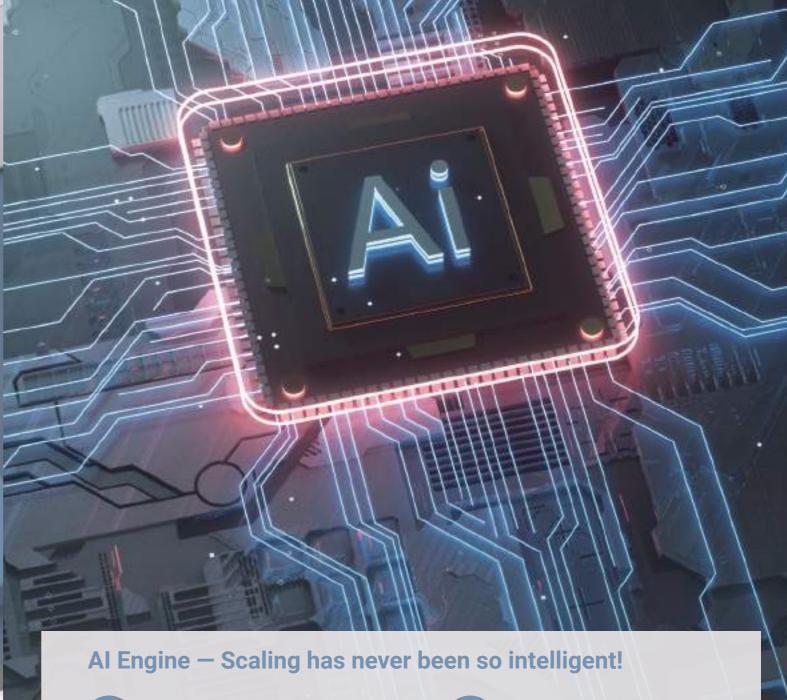



Customized treatment based on tooth surface conditions



Elliptical stroke patterns with polishing effect



Digital controlled automatic frequence tracking

Ensures machine works on

Ensures machine works on optimim frequency



Smart touch control systemultrasensitive & waterproof



Intelligent degenerative feedback



Sine wave drive

Avoids simulation caused by instantaneous current output; ensures comfortable treatment







\*Satelec and EMS are trademarks of Acteon® and EMS®, respectively.

<sup>\*</sup>Satelec a



### CuringPen

4 LEDs curing light

CuringPen

### Technical parameter:

Dimension: 24\*21\*230(mm)


Net Weight: 109g Lens size: 11mm

Power supply: >1200 times, 3 Sec Maximum light intensity




Smart controlling chip keeps light output consistent Light intensity: 1000mw/cm², 1500mw/cm², 2300mw/cm² 600 mw/cm²(detect mode)





Wavelength:385-515nm 3 Blue, 1 Violet, 10w LED







Intensity digital display




Multiple Curing Options

Ramp mode

1000 light intensity(mw/cm²)

0 5 10 15 20 Time(s)



Caries detection







### CuringPen-E

3 LEDs curing light

### **Technical Specifications:**

Dimension : 19 x 16.5 x 7.5 cm

Weight : 120 g Lens Size : 8 mm **Power Supply** 

: >1200 times,

3000 mw/cm<sup>2</sup>, 3 Sec

Maximum Light Intensity : 3000 mw/cm<sup>2</sup> Spectral Range : 380-515 nm



### 360° Rotatable Head

Easy to illuminate various treatment areas



### Small Light Head

Easy to access to posterior molars which offers better patient experience



### Special Lens Design

Unique lens design forms a concentrated beam for uniform curing



### **Ultra Power**

- Light intensity now up to 3000mw/cm<sup>2</sup>
- High light intensity results in deeper cure depths which could curing resins more efficiently and with short time



### Broad Spectral Range 380 nm-515 nm


- Why broad spectral range?
- Most of resins use camphorquinone (CQ) materials, but some manufacturers choose alternative initiators such as TPO to reduce the yellow impact caused by CQ. TPO can only be activated by the light wave below 410nm. CuringPen-E has a broad spectrum which could effectively cure different resins.

•P3

Ultra Mode

### **Working Modes**

•P1



Normal Mode

Light Intensity : 1200mw/cm<sup>2</sup>

Time Setting : 5s, 10s, 15s, 20s, 25s, 30s, 35s, 40s

•P2


(DPE 2 (-)

High Mode

Light Intensity : 2000mw/cm<sup>2</sup> Time Setting : 1s, 3s, 5s, 10s Light Intensity : 3000mw/cm<sup>2</sup> Time Setting : 1s, 3s, 5s

•P4

Eighteeth




Pulse Mode


Light Intensity : 1200mw/cm<sup>2</sup> Time Setting : 5s, 10s, 15s, 20s



Light Intensity : 1200mw/cm<sup>2</sup> Time Setting : 5s, 10s, 15s, 20s







**Eighteeth** 









- Wide temperature range of 90° to 300°
- Five memory programs to customize temperature and cut-off time as per obturation material used or any other intended use of the device

### **Internally Heated Tip**



- Only the working end (4 6 mm) of the tip is heated - avoids need for insulating sleeves
- The non-working end is insulated and stays cool avoiding soft tissue burn





- Fast heating Quick heating prevents PDL damage
- Swift cooling Swift cooling ensure GP does not follow along the heating tip

### **Experience Ergonomics**



- 360° start / stop ring button allows holding the device in any angle comfortable for you
- Left right handed operation
- Comfortable grip, light in weight

### **Powerful Battery**



G

- Highly efficient 2600mAh Lithium battery
- Direct Plug & Play In case of low battery, use the device directly with adaptor

### **Specifications**

Heating Time	0.2 seconds for 200 °C Less than 1 second for 300 °C	
Cooling Time	2 seconds for cooling	
Charging Time	2 hours to complete charge	
Operating Time	4 hours of continuous operation at 250 °C	



Small (Black) 40/0.025 - 1 Qty



Medium (Yellow) 50/0.05 - 1 Qty



Large (Blue) 60/0.06 - 1 Qty



### Fast-Fill

**Obturation Fill** Handpiece

(7) Eighteeth

Fast-Fill



### Fast-Fill Tips

- Autoclavable silver tips for multiple usages
- Silver tips maintain the thermoplastic temperature of GP and offers smooth flow inside canal
- -360 ° rotating tip for easy filling at all angles
- Extra long needle offers convenience and visibility
- Easy to maintain and replace

### Motorized GP Flow



- Provides consistent flow of GP at desirable rate
- Precludes voids and makes obturation homogeneous
- Eliminates hand fatigue that resulted from earlier gun type devices

### Comprehensive Display



- Three customizable memory programs T1 to T3
- Temperature range 100 °C 200 °C
- GP flow rate Low, Medium, High
- Reserve GP level indicator

### Intuitive Design

- Sleek and ergonomic hand-piece
- Simple push button to dispense GP
- LED indicator reflects when the device is ready for use

### Powerful Battery



- Highly efficient 2600mAh Lithium battery
- Direct Plug & Play In case of low battery, use the device directly with adaptor

### Specifications

Heating Time	20 seconds to 200 °C
Charging Time	4 hours to complete charge
Hexagonal Wrench	Use the wrench to bend the tip, rotate the tip and clean the device




23 Gauge



25 Gauge Small





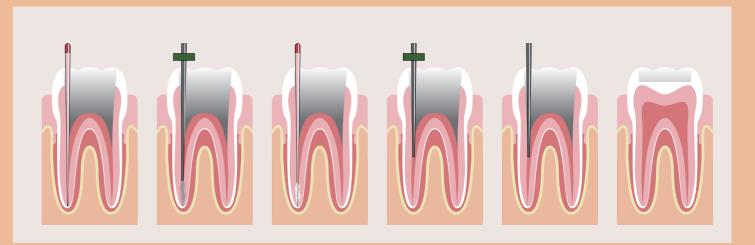

### **Protocol for Use**

### Master Cone Verification & Resizing

Select a master cone which corresponds to the master apical preparation. Check for tug-back and confirm the same with radiograph. Resize the GP by cutting it to 0.5 to 1mm short of the working length. This will prevent peri-apical extrusion of the GP

### Selection of Fast-Pack & Plugger Tip

Select the Fast-Pack tip which reaches 4-5 mm short of the working length and give a snug fit at the tip. Mark this length using the silicon stopper. Similarly, select the hand plugger which reaches 4-5mm short of the working length

### Gutta Percha & Sealer

Coat the master cone apically with the sealer and insert it into the canal. Brush the canal wall using strokes of GP and sealer

### Down Pack with Fast-Pack

Remove the GP from the orifice/coronal part with the help of heated Fast-Pack tip. Plug the GP cone with pre-fit hand plugger at the orifice. Now take the heated Fast-Pack tip 4-5mm short of the working length. The bite of GP will come out of the canal along with the tip. Heated Fast-Pack tip will transfer heat to the GP and convert it into thermoplastic state. Condense the GP with the help of hand plugger to ensure the complete sealing of accessory canals and apex

### Fill with Fast-Fill

Filling the canal using the Fast-Fill device in increments of 4mm till the canal is filled completely while condensing the warm GP with the appropriate plugger after each increment

Fast-Pack pro & Fast-Fill Fast-Pack pro & Fast-Fill S4







### **Integrate Endomotor with Apex Locator** (Connect Function)









### **Smart Accurate and Reliable Apex Locator**

- Advanced Multi frequency Technology
- High Precision in Wet & Dry Canals
- Large 3.5" LCD Display
- Automatic Calibration
- Compact Size & Stable Design

### **Screen Display & Its Meaning**

	Interface	Interface	Interface	Interface
Display	3 2 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1	3		2 - 3 - 3 - 3 - 3 - 3 - 3 - 3 - 3 - 3 -
Value	12	09	00	-3
Meaning	The corresponding scale value is 2, indicating the distance from the apex is about 2mm	It indicate that the distance from the apex is about 1.5mm	It indicates that the endo file reaches the apex	It indicates that the root canal file has exceeded the apex
Alarm	Didi alarm sound for a long time interval	Didi alarm sound interval becomes shorter	Uninterrupted long beep	Very rapid Didi alarm sound

E-PEX E-PEX 36



### AirPex

Wireless Apex Locator

International Patent
No.:PCT/CN2019/110429







### **Feel the Charm of Wireless Charging**

Lay it down , Charge it up Charging is as simple as placing the AirPex on the charging base



### **True Wireless Apex Locator**

Get rid of the wire to the fullest Use without magnet wire Accuracy through wirelessness







- Strong cutting power and stable torque output
- 4 memory program presets monitor speed and direction
- 4 transmission ratio presets offer the versatility to choose the right system to fit your treatment needs
- LCD touch screen and color display provide an intuitive user interface to reduce time spent making adjustments
- The standard four-hole connector of main unit suitable for all types of dental chairs
- Reliable security alarm system





Light intensity adjustment



Foward/ Reverse



Memory programms switching (M1-M4)



Speed adjustment



Transmission ratio presets (1:5 1:1 16:1 20:1)



### Long-lasting brushless motor with a cooling system

### - More comfortable

A strong cooling system provides patients with a comfortable temperature in treatment

### Longer lifetime

Brushless DC motor lifespan is approximately 6 times higher than the counter brushed DC motor

### Quieter

Produce comparatively low operating noise as compared to other motors of the same ratings

### More efficient

A very compact and small-sized brushless DC motor provides maximum torque continuously during rotation

Motorturbo & F-Asp 1 Motorturbo & F-Asp 1







### LED fiber optics

- Shines light directly during the preparation, improving visibility tremendously Reduces visual fatigue and stress



### Durable components

- Achieve long-lasting performance through repeated sterilization



### Ergonomic design

Enhances grip for better control



### Multi-port spray

Keeps the bur cool while whisking debris



### Super strong push button chuck system

- Enhanced bur retention and long-lasting reliability
- Time saving and quick bur change

### Specifications

Electric Motor		High-speed Handpiece		
Model	MotorTurbo	Model	E-ASP1	
Display	LCD colour display	Maximum allowable	40000 rpm	
Dimension main unit	130 x 129x 54 mm	motor speed(rpm)		
Weight	600 g	Ratio	1:5	
Memory programms	M1-M4	Motor connector	Comply with ISO 3964	
Transmission ratio presets	1: 5 1: 1 16: 1 20: 1	Chuck type	Push-button chuck	
Motor speed range	2000-40000 rpm	Bur dimension	Bur shank Ø 1.6 m	
Motor torque	Max. 3.0 Ncm	Optical fiber	Light guide glass	
Power cable length	1.5 m	Cleaning/Sterilisation	Steam autoclave	
Motor tail wire length	2 m	Oleaning/Stermsation	up to 135°C	





### **Engineered for accurate images**

- Clinical Imagery








- Sharp, high resolution images with a 0.4 focal spot

Source focal spot Source focal spot





Effect of focal spot size



### **Designed with safety in mind**



Built-in leaded double shield to protect the operator from leakage radiation



Locking system to prevent unintentional exposure

### **Specifications**

Model	HyperLight	Weight	1.8 kg
Focal Spot	0.4	Battery	2500 mAh x 4
Tube Voltage	65 kV	Exposure Time Range	0.02-2 Sec
Tube Current	2.5 mA	Line voltage	100V-240V, 50Hz/60Hz

HyperLight 44







### Simplify your digital workflow

- Compact size and lightweight can make you operate it by one hand only
- Intuitive user interface
- Smart angulation system











HyperLight HyperLight 46



### HyperLight-G

Portable X-ray unit







### Receptor

Use with film, digital sensor, phosphor plate



### Locking System



### **Preset Parameter**

Divided into adults and children, and can be set and controlled for different teeth



### **Large Battery Capacity**

More than 300 exposures in one full charge



Smart angulation system, faster your workflow



### Safe

- Internal x-ray shielding
- Locking system to avoid unintentional exposure
- Backscatter shield for operator and patient protection(\*optional)

### **Portable**


 Cordless, handheld and extremely mobile, move freely between rooms, locations and cities

### Economical

- Use with film, digital sensor or phosphor plate
- Prolonged working life, at least 80,000 exposures

### **Specifications**

Model	HyperLight-G	
Tube Voltage	65 kV	
Tube Current	2 mA	
Exposure Time Range	0.02-2 Sec	
Weight	1.9 kg	
Battery	2000mAh X4	
Line Voltage	100V-240V, 50Hz/60Hz	

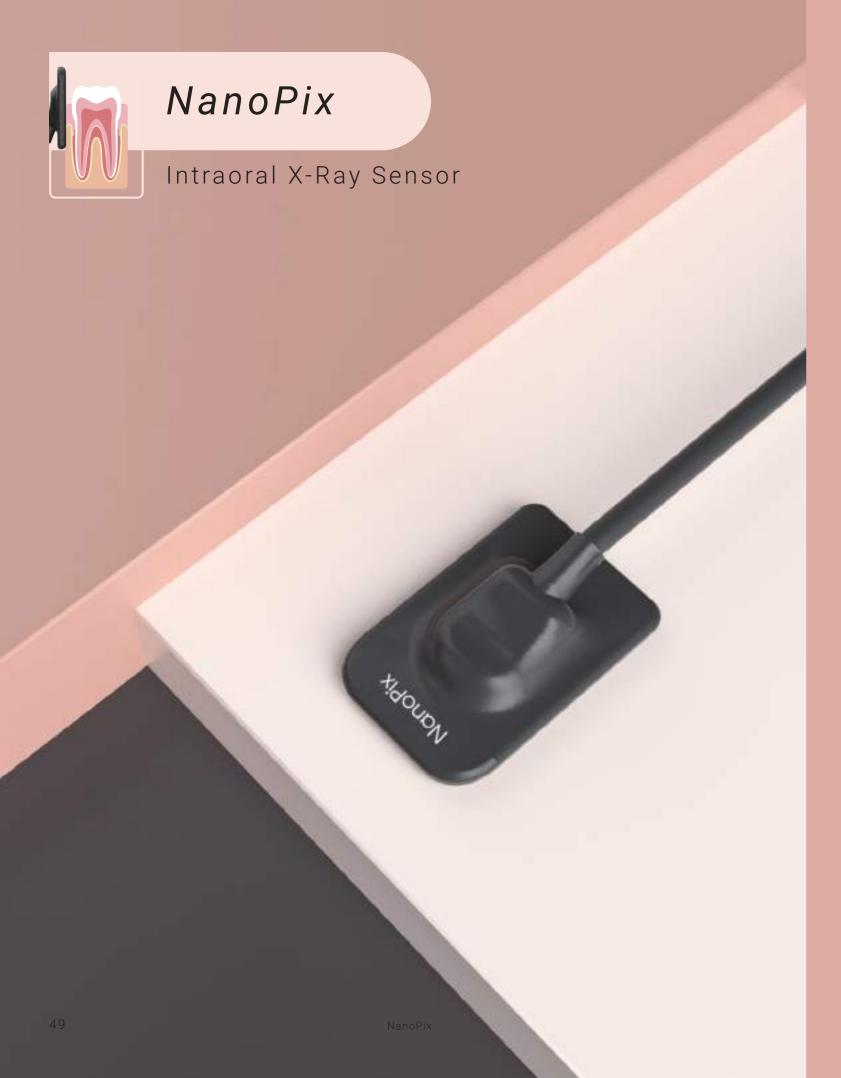



1/10 Cost per patient compared to film 3s To complete entire imaging process 50000+ Exposures with no quality loss



### **Leading technologies : The 1st time in dentistry**



### AED Technology (Automatic Exposure Detection)

- from chest radiography
- Compatible with almost all DC and AC X-Ray generators
- Digital images comes automatically when your X-Ray is switched on



### APS CMOS Technology

from aerospace industry

- High signal-to-noise ratio with maximum details
- Long life and low power consumption



### Direct Deposition CSI Technology

- from chest radiography
- Low dose radiation for safety
- Less exposure time but higher resolution

All-in-one The most economical X-Ray sensor in the world



### **Unique design**



### Ergonomic design

Cupped cable connection ensures comfortable finger positioning



### Robust cable connection

70000+ Bendings RA test passed



### Ultra-thin body design

4.4mm - the thinnest X-Ray sensor

### **Easy-of-Use software with only**

### 4 steps

• Step 1. Choose 'Patient'



Step 3. View Image




• Step 2. Image 'Acquisition'



Step 4. Generate 'Report'



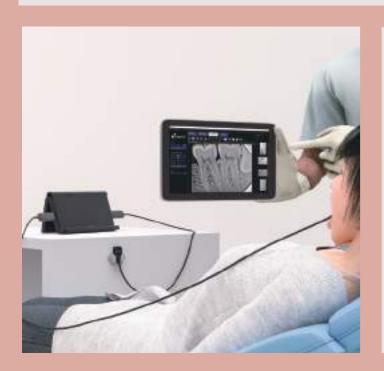

### **The Complete Image Solution:**

excellent combination of DR Pad & its base



pre-installed software



multiple USB ports for diverse needs




build an instant connect with users



### **Specifications(available in 2 sizes)**

	NanoPix 1	NanoPix 2
Detector Technology	APS CMOS	APS CMOS
Scintillator	Csl	Csl
Pixel Matrix	1000*1500	1300*1800
Theoretical Resolution	25lp/mm	25lp/mm
True Resolution	20lp/mm	20lp/mm
Active Area (mm)	20*30	26*36
Mechanical Size(mm)	25.4*36.8*4.4	30.4*41.9*4.4
AD Conversion(bit)	16	16
Data Interface	USB 2.0	USB 2.0
Protection	IP68	IP68

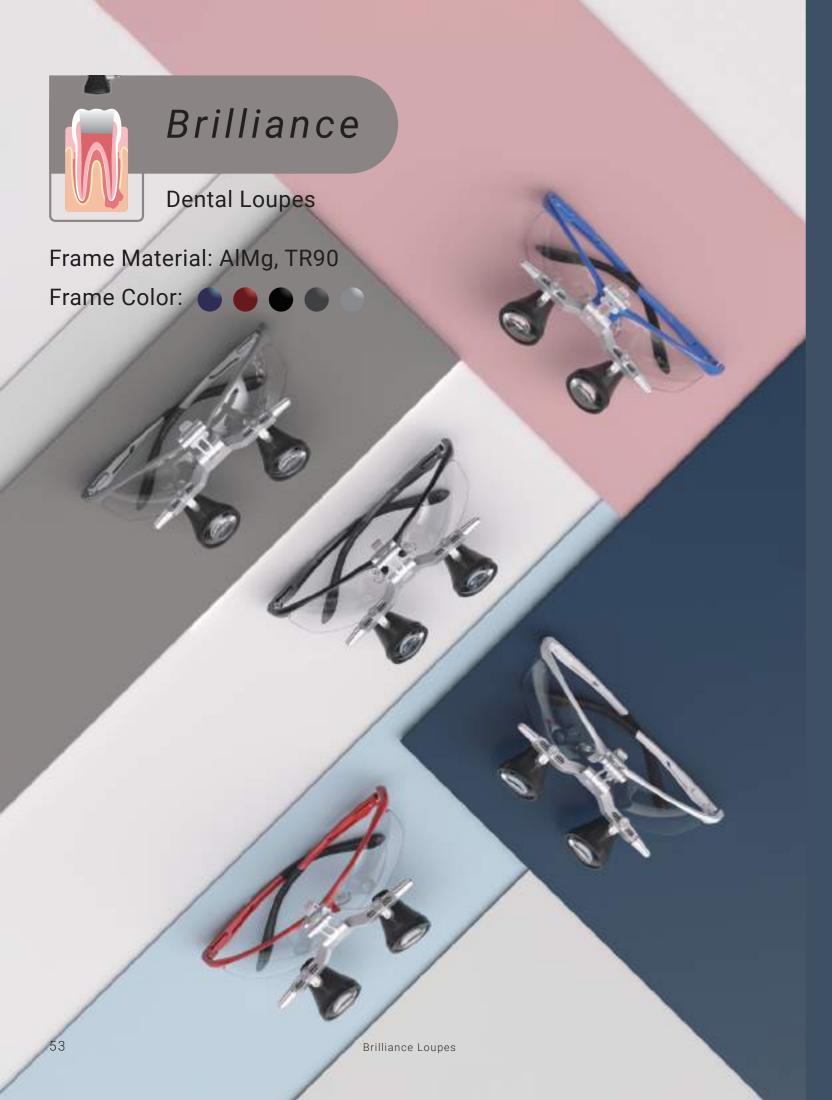



### Lens

-Schott Glass

Ensure high resolution, clear and sharp field of view

Refined lens coatings

Multi-layer coating technology, Anti-fog, Anti-scratch, Anti-glare, to ensure more visible light through the glass



### Body

- Aerospace-grade aluminium magnesium alloy
   Our loupes are exceptionally high strength and light
- Intelligent damping torque effect
- Easy to adjust and with excellent stability

   Asynchronous PD adjustment

Laser printed scale lines, accurate and intuitive



### Frame

-Super light frame

Ergonomic design with optional materials and colors

- Protective shield

Besides protective shields, prescription lenses can also be fitted by an optometrist



### **Two Options**

Both can be quickly and accurately reset after flipped-up without extra adjustment. Get into the next use immediately, and greatly improve the work efficiency.

### Two hinges type





### Three hinges type







### Your ideal first pair of Loupes!

Magnification	Working Distance	Field of View	Depth of Field	Net Weight
	350mm	68mm	≥90mm	71g
3.0×	400mm	76 mm	≥100mm	71g
	450mm	84mm	≥115mm	71g
	500mm	92mm	≥135mm	71g

Brilliance Loupes 54



### **Specifications**

Lamp Diameter	18.5 mm	Battery Type	Li-lon
Lamp Length	36.5 mm	Battery Capacity	3350 mAh, 3.7 V
Lamp weight	8 g	Charging Time	4 hours
Brightness	35000 lux	Battery Life	≥11 hours (with maximum brightness)
Color Temperature	5000 k	Adapter Input	100-240 V, 50/60 Hz, 0.2 A
CRI	90	Adapter Output	5 V, 1 A
Power	1 W	Power Box Weight	145 g





### Super Light

Made by aviation grade alunminum, only weighs 8g.



### **Top Class Light Source**

True color, and máximum brightness up to 35000 Lux.



### **Ultra-long Battery Life**

Can keep illuminating for 11 hours with maximum brightness.



### Safe to Use

High-level short-circuit and open-circuit protection.
Power box clip to belt or pocket.



### Touch Control Design and Stepless Dimming

Touch botton clip to collar or chest pocket, avoid shaking



Short touch to turn on/ off the light, long press to adjust steplessly the brightness.


Wired headlight reduces the weight on the bridge of the nose, providing dentists a durable and comfortable experience.

### CRI 90

Reveal true color, and improve safety as a result of increased visibility








### **Color Temperature 5000K**

Close to the color temperature of sunlight, can reduce eye fatigue in long surgery



### Edge to Edge Clarity, and Flicker Free

Fascinating optical design and high quality light-source make the light spot more uniform and soft

Flicker free avoids eye fatigue after long-time usage, and limits the damage to eyes.







Manufactur

Manufacturer B

Softouch Softouch Softouch

### UltraClean

**Antibacterial Root** Canal Cleanser






Use Ultra Clean replace EDTA to After all preparations are moisturize the root canal before completed, each root canal is used 5ml Ultra Clean. preparation. It can lubricate and Use the side opening irrigation needle to pull-up rinse at the 1mm from apex. debris removal. When preparing and changing files, use Ultra Clean to kill bacteria and remove

Activate Ultra Clean 20 seconds by Ultra X (Low power mode) to remove smear layer better. Ultra Clean will enters the dentin tubules and kill the bacteria.

Use UltraMint /UltraMint Pro tips (or side opening irrigation needle) maximum volume irrigation solutions. The debris and smear layer will be rinsing out. It can be used as a final rinse.

Caution: Do not mix with CHX solution!

### Comparison of the effect of 5.25% NaClO and Ultra Clean

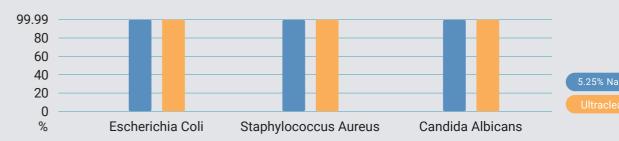

**Conclusion** — Ultra Clean has the same bactericidal effect as 5.25% NaClO


### Effectively remove the smear layer



**Conclusion** — Ultra Clean is as effective as 17% EDTA to remove smear layer. At the same time, Ultra Clean can clean the dentin and dentin tubules underneath without corroding the dentin.

### **Explanation of Principle**


- Benzalkonium Chloride achieves bactericidal effect by destroying the bacterial cell wall.
- When the external concentration of Benzalkonium Chloride decreases, it could be released slowly and has a slow-release bactericidal effect.
- As a chelating agent, Sodium Citrate could remove smear layer.




### **Comparison Data**

	Ultra Clean	MTAD	2% CHX	5.25% NaCIO	17% EDTA
Main Ingredients	Sodium Citrate BAC	Citric Acid Doxycline	CHX	NaClO	EDTA
Dentin Erosion	No	Yes	No	No	Almost No
Dentin Discoloration	No	Yes	Yes	No	No
Bactericidal Effect	Strong	Strong	Strong	Strong	Weak
Smear Layer Removal	Yes	Yes	No	No	Yes
Safety	Very Safe	Safe	Safe	Dangerous	Very Safe
Smell	Good	Bad	Not Good	Bad	Not Good
Cost	Low	High	Low	Low	Low


destroy bacteria

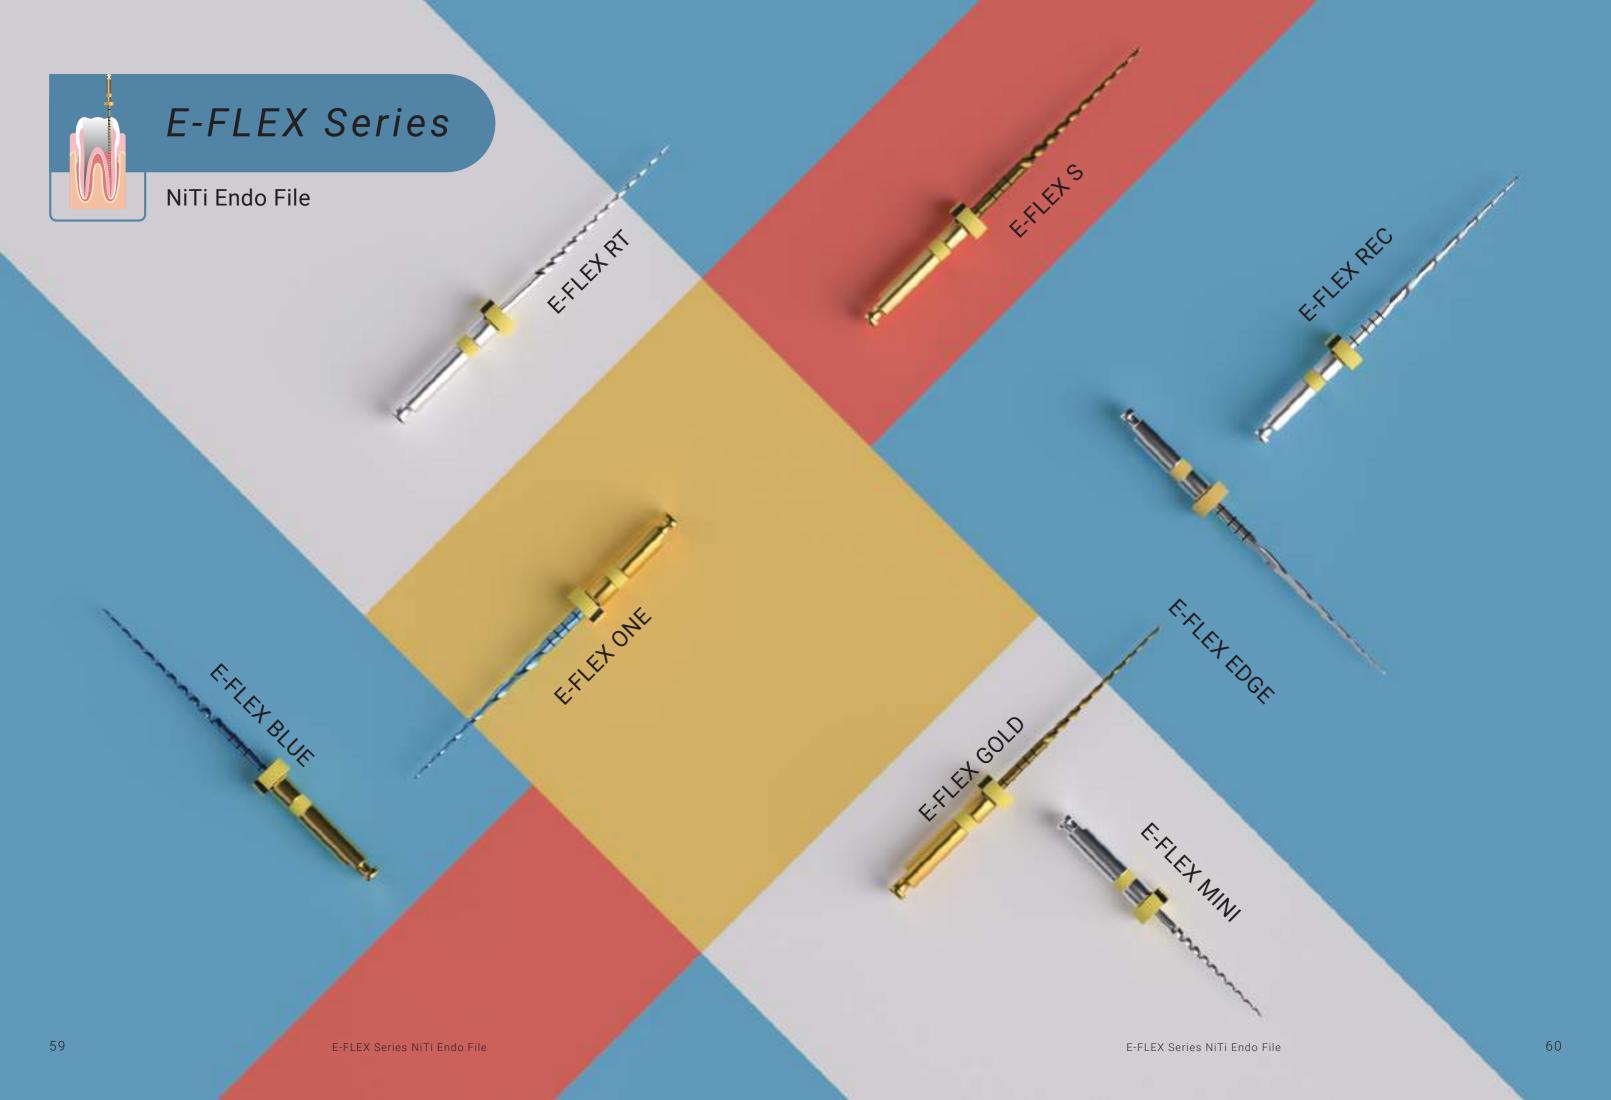

### **E-FLEX GOLD**

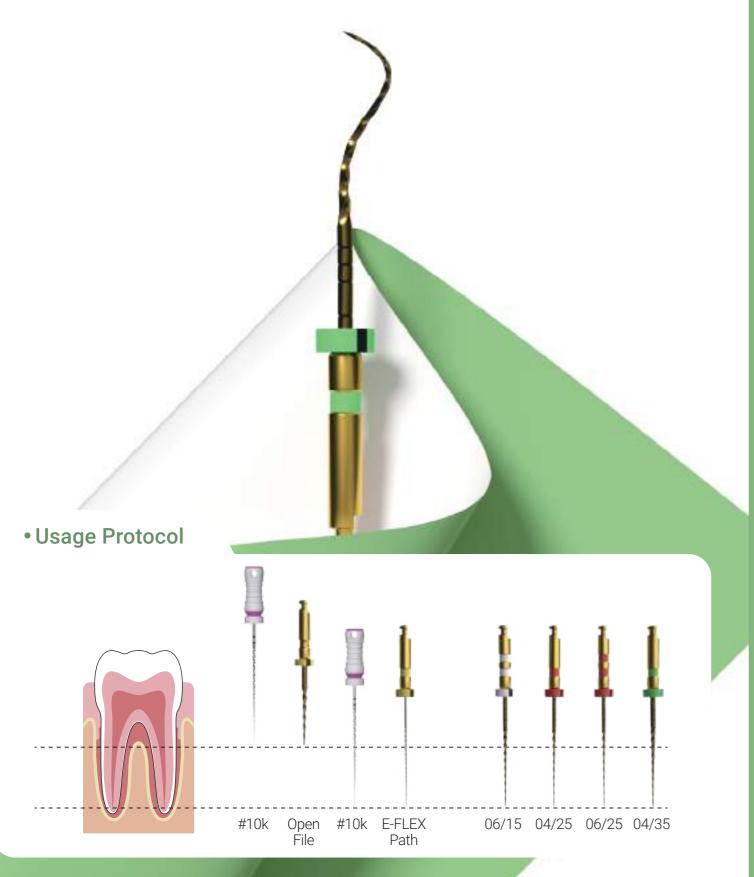


### Gold Heat Treatment allows safe navigation of any curved canal

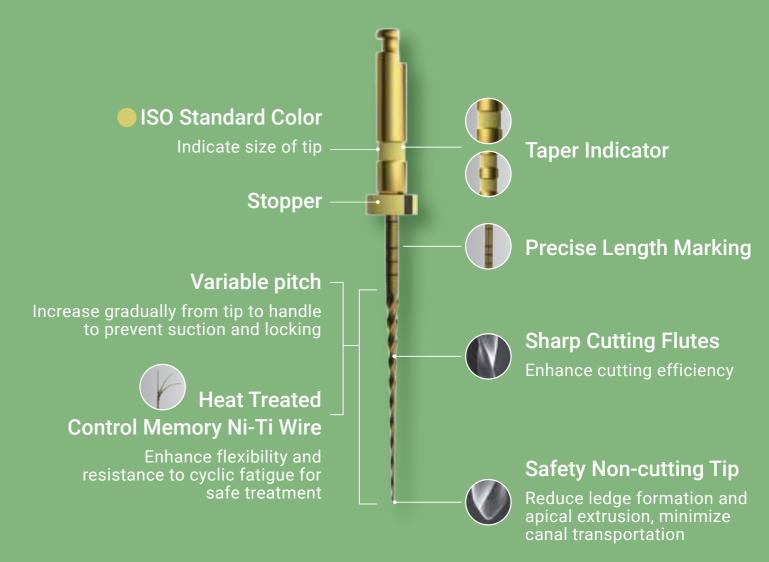


	Color	Tip Size	Taper (%)	Taper Indicator	Cross-Section	Length (mm)	Suggested Speed/ Torque
		17	8	100		19	300 rpm, 3 N·cm
	0	15	4				
		20	4	-86-			
		25	4				350 rpm 2.5 N·cm
		30	4	- E			
E-FLEX		35	4			21/25/31	
GOLD	0	15	6				
		20	6	No.			
		25	6				
		30	6	10 20			
		35	6	*****			




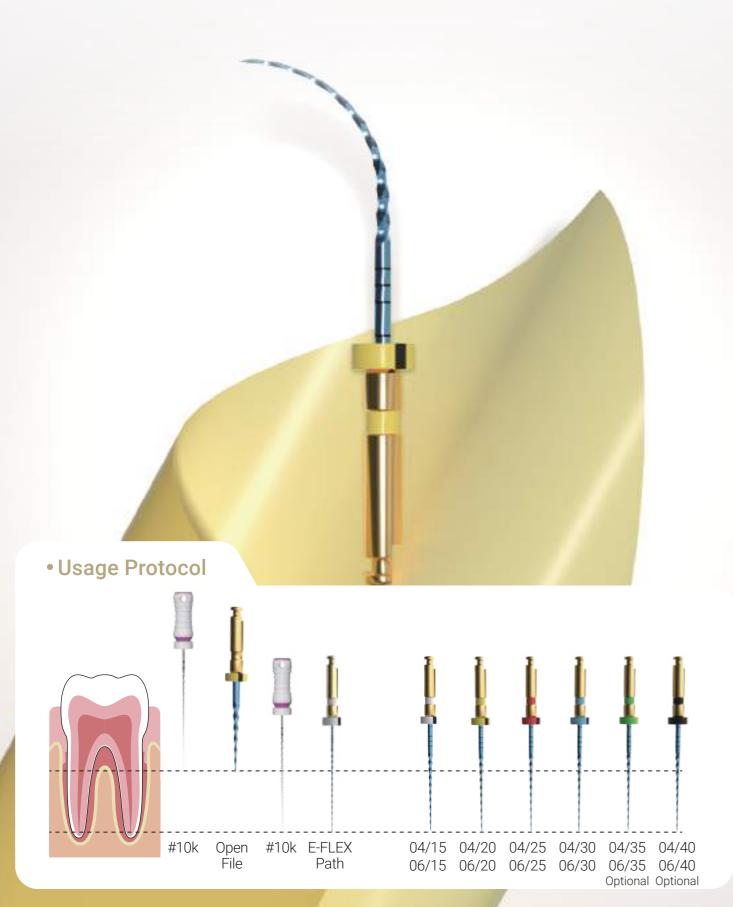


Blue Heat Treatment provides superior strength while maintaining flexibility to negotiate all canals

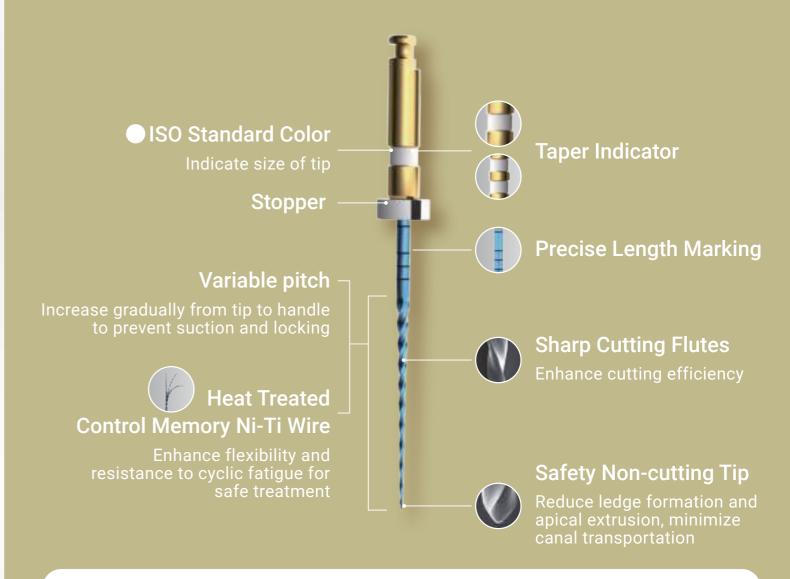

	Color	Tip Size	Taper (%)	Taper Indicator	Cross-Section	Length (mm)	Suggested Speed/ Torque
		17	8	100		19	300 rpm, 3 N·cm
	0	15	4				
		20	4	-80			
		25	4				
		30	4			]	
E-FLEX		35	4				350 rpm
BLUE	•	40	4	-		21/25/31	2.5 N·cm
BLUL	0	15	6				
		20	6	No. of Concession, Name of Street, or other party of the last of t			
		25	6				
		30	6			]	
		35	6				
	•	40	6	8-9			

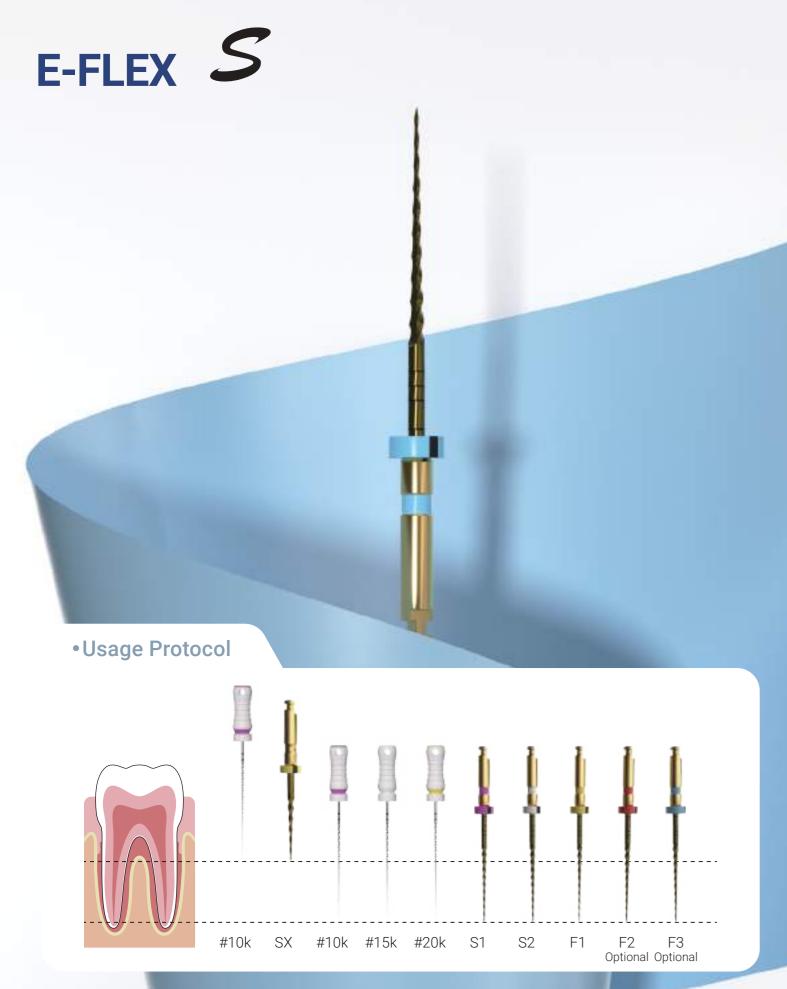


- 3 Shaping files for a deep shape
- 3 Finishing files for navigating challenging curves in the apical region

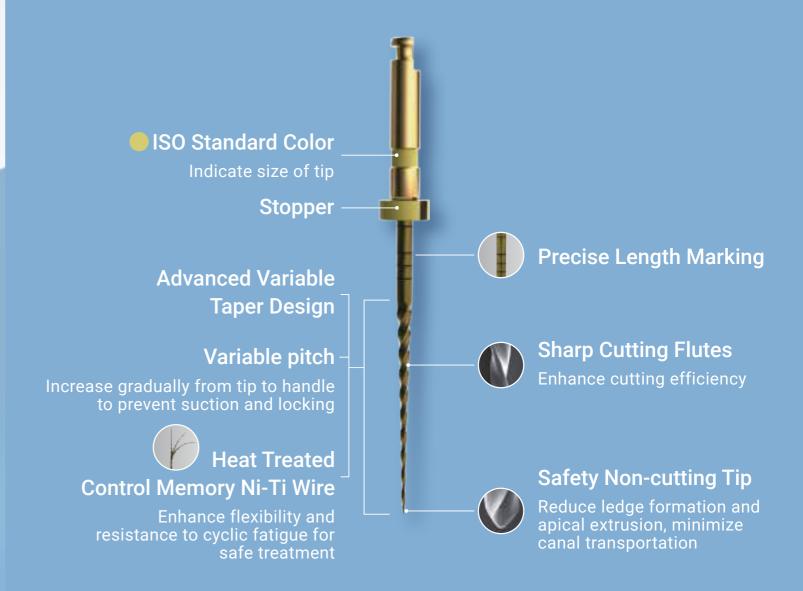

	Color	Tip Size	Taper (%)	Cross-Section	Length (mm)	Suggested Speed/ Torque
	•	16			19	
	•	18				
E-FLEX	0	20	Variable			350 rpm
S		20	Taper		21/25/31	2 N·cm
	•	25				
	•	30				

# Different heat treatments are available: E-FLEX EDGE Silver/ Gold / Blue Variable pitch Increase gradually from tip to handle to prevent suction and locking Stopper Stopper

# Variable pitch Increase gradually from tip to handle to prevent suction and locking Stopper Taper Indicator Safety Non-cutting Tip Reduce ledge formation and apical extrusion, minimize canal transportation Indicate size of tip Flat-sided Design More room for bypass and debris remove, significantly decrease screwing effect Precise Length Marking

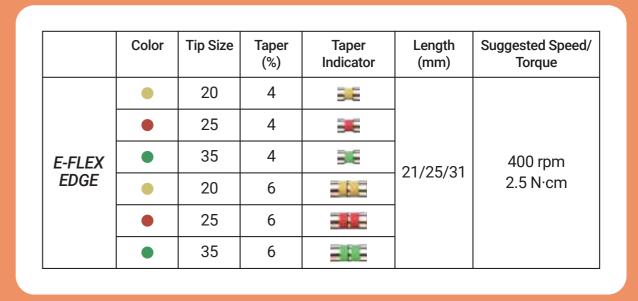

68

Usage Protocol

#10k

Open

File

#10k

04/20 04/25 04/35


06/20 06/25 06/35

## E-FLEX ONE Usage Protocol #10k Open #10k E-FLEX 04/20 04/25 04/35 File Path 06/20 06/25 06/35

One file for incredible efficiency
Blue Heat Treatment for increased flexibility and safety




	Color	Tip Size	Taper (%)	Taper Indicator	Cross-Section	Length (mm)	Suggested Speed/ Torque
		20	4	-			
	•	25	4				
E-FLEX	•	35	4			01/05/01	400 rpm
ONE		20	6			21/25/31	2.5 N·cm
	•	25	6				
	•	35	6	11.40			

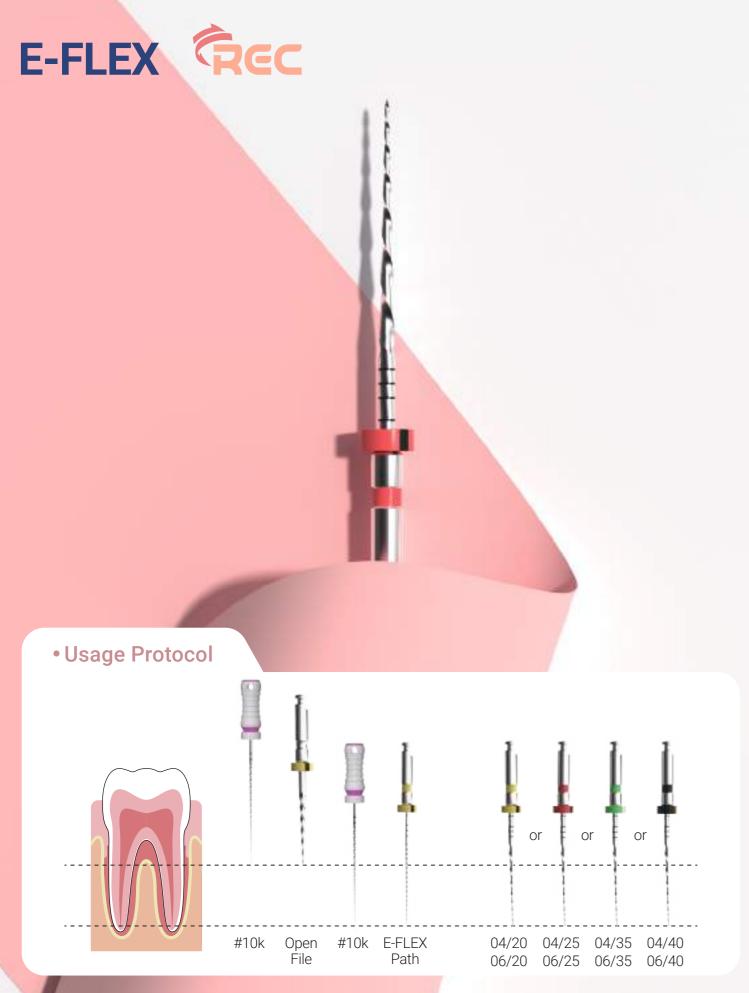

One file reciprocation for incredible efficiency





**Taper Indicator** 

Precise Length Marking

Sharp Cutting Flutes
Enhance cutting efficiency

Double S Cross-Section

Efficient removal of debris


Safety Non-cutting Tip

Reduce ledge formation an apical extrusion, minimize canal transportation

	Color	Tip Size	Taper (%)	Taper Indicator	Cross-Section	Length (mm)	Suggested Angle
		20	4	89			
	•	25	4	9			
	•	35	4			21/25/31	FWD: 30°
E-FLEX	•	40	4				
REC		20	6		21/25/	21/23/31	REV: 150°
	•	25	6				
		35	6				
	•	40	6	777			

# E-FLEX MINI Usage Protocol

### For deciduous teeth

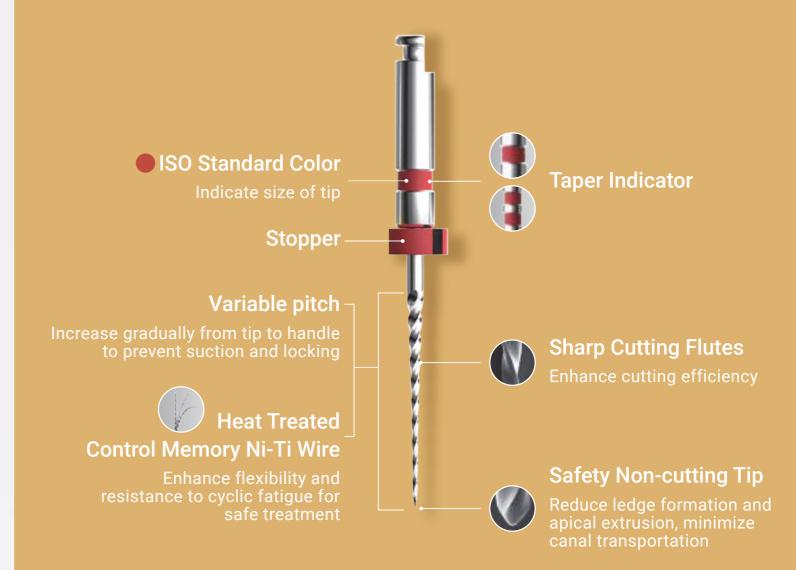

	Color	Tip Size	Taper (%)	Taper Indicator	Cross-Section	Length (mm)	Suggested Speed/ Torque
		17	8	Ħ		10	300 rpm, 3 N·cm
		20	4	35			
		25	4				
E-FLEX MINI	•	30	4			16	350 rpm 2.5 N·cm
		20	6			10	
	•	25	6				
	•	30	6				

#10k Open #10k

File

04/20 04/25 04/30

06/20 06/25 06/30



	Color	Tip Size	Taper (%)	Taper Indicator	Cross-Section	Length (mm)	Suggested Speed/ Torque
	•	13	2	300			350 rpm 2.5 N·cm
E-FLEX		16	2	500		01/05/01	
PATH		19	2	-		21/25/31	
	•	15	3	575			


### Advantages over the manual file

- Intensive flexibility and more resistance to cyclic fatigue
- Follow the contour of root canal, retain more dentin
- Shorten preparation time significantly
- Less canal transportation
- Suitable for curved canals

Reduce ledge formation and apical extrusion, minimize canal transportation

**Safety Non-cutting Tip** 



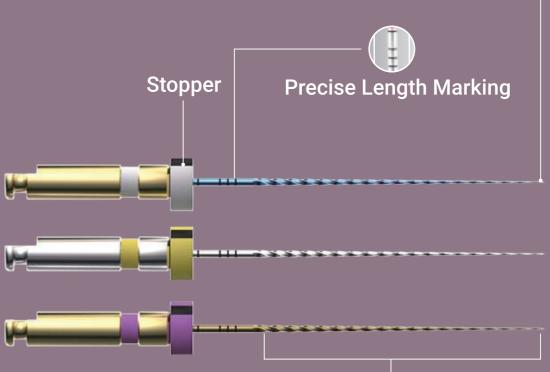

### Variable pitch

Increase gradually from tip to handle to prevent suction and locking



### Heat Treated Control Memory Ni-Ti Wire

Enhance flexibility and resistance to cyclic fatigue for safe treatment

Different heat treatments are available: E-FLEX PATH Silver/ Gold / Blue

76

### E-FLEX RT

### Usage Protocol For Coronal 1/3 09/30 For Middle 1/3 08/25 For Apical 1/3 07/20

### Safe and effective removal of obturation materials Reducing the need for solvents



	Color	Tip Size	Taper (%)	Cross-Section	Length (mm)	Suggested Speed/ Torque
	•	30	9		16	
E-FLEX RT	•	25	8		18	350 rpm 2 N·cm
	•	20	7		22	