



DS Implants™

DS OmniTaper™  
Surgical product catalog



All Dentsply Sirona Instructions for Use are available on [www.dentsplysirona.com/ifu](http://www.dentsplysirona.com/ifu)

All products may not be regulatory cleared/released/licensed in all markets. Please contact the local Dentsply Sirona sales office for current product assortment and availability.

To improve readability for our customers, Dentsply Sirona does not use ® or ™ in body copy. However, Dentsply Sirona does not waive any right to the trademark and nothing herein shall be interpreted to the contrary.

Product illustrations are not to scale.

# CONTENTS

<b>1. Implant packaging</b>	4
Color coding	4
<b>2. Implants</b>	5
<b>3. Cover Screw</b>	6
<b>4. TempBase Cap</b>	6
<b>5. Healing abutments</b>	6
<b>6. Instruments</b>	9
Initial drills	9
Drills	9
Taps	10
Implant drivers	11
Planning aids	12
Torque Wrench	13
Driver	13
Surgical Trays	14
Washtray & Overlay	16
Sterilization Container & Reusable Filter	17
<b>7. Guided Surgery Instruments</b>	18
Punch	18
Drills	18
Taps	20
Sleeves	21
Driver	21
Sleeves for Driver	21
Stabilization Abutment	22
Positioning Aid	22
Surgical Trays	22
<b>8. Material specifications</b>	25
<b>9. Index</b>	26

# 1. Implant packaging

DS OmniTaper implants are supplied in a double-blister package with an outer carton.



## Outer box

- Specific color coding, diameter and prominent implant length information on side labels
- Data matrix code on two sides
- Stackable, with all important product information visible
- Instructions For Use (IFU) available electronically (eIFU): [ifu.dentsplysirona.com](http://ifu.dentsplysirona.com)



## Outer blister

- Peel-off label with batch code for convenience treatment documentation



## Inner blister

- Inner sterile package
- Implant shuttle with implant and cover screw
- Peel-off label with batch code for convenience treatment documentation

## Color coding

The DS OmniTaper implant is available in five diameters and six lengths. The color coding makes it easy to identify the correct connection and to select the right prosthetic components.

Implant Ø	3.0mm	3.4mm	3.8mm	4.5mm	5.5mm
Connections	<b>XS</b>	<b>S</b>	<b>M</b>	<b>L</b>	<b>XL</b>
Lengths	-	-	8mm	8mm	8mm
	-	9.5mm	9.5mm	9.5mm	9.5mm
	11mm	11mm	11mm	11mm	11mm
	13mm	13mm	13mm	13mm	13mm
	15mm	15mm	15mm	15mm	15mm
	-	18mm	18mm	18mm	-

## 2. Implants

### XS OmniTaper EV Ø3.0



Length mm	11	13	15
Order No.	68011140	68011141	68011142

### S OmniTaper EV Ø3.4




Length mm	9.5	11	13	15	18
Order No.	68011143	68011144	68011145	68011146	68011147

### M OmniTaper EV Ø3.8



Length mm	8	9.5	11	13	15	18
Order No.	68011148	68011149	68011150	68011151	68011152	68011153



### L OmniTaper EV Ø4.5



Length mm	8	9.5	11	13	15	18
Order No.	68011154	68011155	68011156	68011157	68011158	68011159

### XL OmniTaper EV Ø5.5



Length mm	8	9.5	11	13	15
Order No.	68011160	68011161	68011162	68011163	68011164

### OmniTaper EV implant

Titanium<sup>1</sup>, Titanium alloy<sup>2</sup>, sterile

The DS OmniTaper implant is designed for replacing one or more missing teeth in order to restore chewing function.

- Endosseous section with OsseoSpeed surface
- Compatible with EV Prosthetics assortment
- Restoration: Various possibilities for type of fixation e.g., screw-, cement-, friction- and attachment-retained solutions. For one-position-only, six-position and non-indexed abutments
- Clinical use: one-stage or two-stage surgical procedures
- Premounted multifunctional TempBase that serves as a placement head, index impression and basis for temporary restorations
- Color coded
- Contains: Implant, Placement head (TempBase), Cover Screw
- Instruments needed: Implant Driver TempBase or optional Implant Driver EV

### 3. Cover Screw











#### Cover Screw EV

Titanium alloy<sup>2</sup>, sterile

The Cover Screw is used for sealing the implant interface.

- Clinical use: two-stage surgical procedures
- Color coded

#### Cover Screw EV

					
					
Order No.	68010001	68010002	68010005	68010006	68010007





### 4. TempBase Cap

#### TempBase Cap

Polypropylene<sup>3</sup>, non-sterile

The TempBase Cap is used for index registration during surgery and basis for temporary restorations.

#### TempBase Cap

			
			
			
			
Order No.	68010013		68010014
			68010015


### 5. Healing abutments

#### HealDesign™ EV







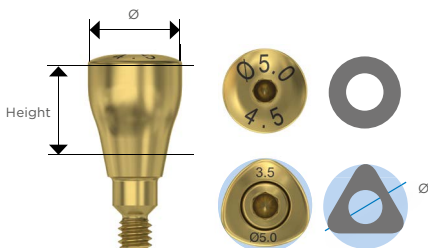

Titanium alloy<sup>2</sup>, sterile

The HealDesign EV is used for soft tissue sculpturing during the healing phase.

- Marked with diameter and height
- Clinical use: one-stage or two-stage surgical procedure
- Round shapes are indicated for all positions in the mouth
- Triangular shapes for anterior implant sites to mimic the incisors and canines
- Triangular HealDesign EV is a two-piece abutment
- Color coded



#### HealDesign EV

				
				
∅ mm	3.5	3.5	3.5	3.5
Height mm	2.5	3.5	4.5	6.5
Order No.	68013001	68013002	68013003	68013004

**S** HealDesign EV



Ø mm	4	4	4	4	5	5	5	5	6	6	5
Height mm	2.5	3.5	4.5	6.5	2.5	3.5	4.5	6.5	3.5	4.5	3.5
Order No.	68013005	68013006	68013007	68013008	68013009	68013010	68013011	68013012	68013013	68013014	68013039

**M** HealDesign EV




Ø mm	5	5	5	5	6.5	6.5	6.5	6.5	5	6.5
Height mm	2.5	3.5	4.5	6.5	2.5	3.5	4.5	6.5	3.5	3.5
Order No.	68013015	68013016	68013017	68013018	68013019	68013020	68013021	68013022	68013040	68013041

**L** HealDesign EV



Ø mm	5	5	5	5	6.5	6.5	6.5	6.5	7.5	7.5	5	6.5
Height mm	2.5	3.5	4.5	6.5	2.5	3.5	4.5	6.5	3.5	4.5	3.5	3.5
Order No.	68013023	68013024	68013025	68013026	68013027	68013028	68013029	68013030	68013031	68013032	68013042	68013043

**XL** HealDesign EV




Ø mm	6.5	6.5	6.5	6.5	7.5	7.5
Height mm	2.5	3.5	4.5	6.5	3.5	4.5
Order No.	68013033	68013034	68013035	68013036	68013037	68013038

### Healing Abutment EV


Titanium alloy<sup>2</sup>, sterile

The Healing Abutment EV is used for soft tissue sculpturing.

- Laser-etched bands for gauging
- Marked with diameter
- Color coded

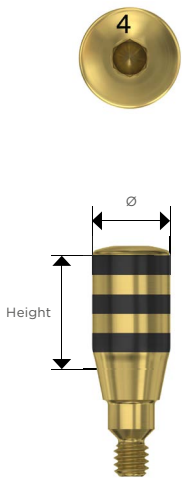

#### XS Healing Abutment EV



Ø mm	4	4	4	4
Height mm	2	3	4	6
Order No.	68013044	68013045	68013046	68013047

#### S Healing Abutment EV



Ø mm	4	4	4	4
Height mm	2	3	4	6
Order No.	68013048	68013049	68013050	68013051

#### M Healing Abutment EV



Ø mm	4	4	4	4
Height mm	2	3	4	6
Order No.	68013052	68013053	68013054	68013055

#### L Healing Abutment EV



Ø mm	4.3	4.3	4.3	4.3
Height mm	2	3	4	6
Order No.	68013056	68013057	68013058	68013059

#### XL Healing Abutment EV



Ø mm	4.8	4.8	4.8	4.8
Height mm	2	3	4	6
Order No.	68013060	68013061	68013062	68013063



## 6. Instruments

Guide Drill



Precision Drill



Order No.	68015133	68015134
-----------	----------	----------

All drills except the Precision Drill can be used for maximum ten cases. They should be carefully cleaned and sterilized after each surgery and replaced as soon as a decrease in their cutting efficiency is observed.

### Initial drills

#### Guide Drill

Stainless steel<sup>1</sup>, sterile

The Guide Drill is used for marking and to create a starting point.

- Multiple use

#### Precision Drill

Stainless steel<sup>1</sup>, sterile

The Precision Drill is used for marking and to create a starting point.

- Single use

The Precision Drill is an extremely sharp drill and should be handled with caution to avoid injury.

### OmniTaper Drill short



Ø mm	2.0	3.0	3.4	3.8	4.5	5.5
Color coding						
Order No.	68015098	68015099	68015100	68015101	68015102	68015103

### OmniTaper Drill long



Ø mm	2.0	3.0	3.4	3.8	4.5	5.5
Color coding						
Order No.	68015086	68015087	68015088	68015089	68015090	68015091

### Drills


#### OmniTaper Drill

Stainless steel<sup>1</sup>, TiN-coated<sup>2</sup>, sterile

The OmniTaper Drill is used for implant site preparation.

- Two-edged profile
- Multiple use
- Depth marked
- Color coded

Drill short 8-15mm  
Drill long 8-18mm

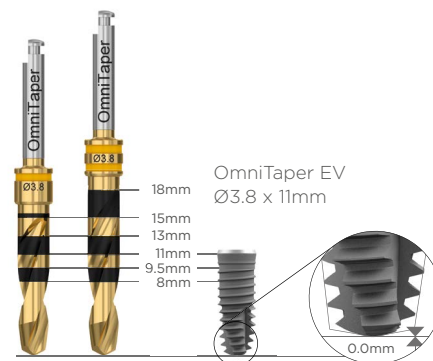

The effective drill depth matches the implant length.

### OmniTaper Single Patient Drill

Stainless steel<sup>1</sup>, ABS<sup>2</sup>, sterile

The OmniTaper Single Patient Drill is used for implant site preparation.

- Single use
- Depth marked
- Color coded
- Available in short L 8-15mm

### OmniTaper Single Patient Drill




Ø mm	2.0	3.0	3.4	3.8	4.5	5.5
Color coding						
Order No.	68015080	68015081	68015082	68015083	68015084	68015085

### OmniTaper Crestal Drill

Stainless steel<sup>1</sup>, TiN-coated<sup>3</sup>, sterile

The OmniTaper Crestal Drill is used for crestal implant site preparation according to the bone quality once the planned implant diameter has been reached.

- Multiple use
- Depth marked
- Color coded



### OmniTaper Crestal Drill



Ø mm	3.0	3.4	3.8	4.5	5.5
Color coding					
Order No.	68015092	68015093	68015094	68015095	68015096


## Taps

### OmniTaper Tap

Stainless steel<sup>1</sup>, sterile

The OmniTaper Tap is used for additional tapping in cortical bone (D I).

- Multiple use
- Color coded
- Instruments needed: contra-angle with HXSS connection or torque wrench with surgical driver handle

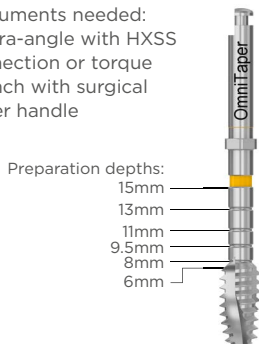

### OmniTaper Tap



Ø mm	3.0	3.4	3.8	4.5	5.5
Color coding					
Order No.	68015104	68015105	68015106	68015107	68015108

### Implant Driver TempBase



Order No.	68015129	68015130
-----------	----------	----------

### Implant Driver TempBase O-Ring



Order No.	68015131
-----------	----------

### Implant Driver EV short



Ø mm	3.4	3.8	4.5	5.5
Color coding				
Order No.	68015188	68015190	68015192	68015194

### Implant Driver EV long



Ø mm	3.0	3.4	3.8	4.5	5.5
Color coding					
Order No.	68015187	68015189	68015191	68015193	68015195

## Implant drivers

### Implant Driver TempBase

Stainless steel<sup>1</sup>, EPDM<sup>2</sup>, non-sterile

The Implant Driver TempBase is used for installing OmniTaper implants with the TempBase (standard procedure).

- Dimple to facilitate correct positioning
- Applicable for all implant diameters
- Available in short/long
- Multiple use
- Instruments needed: contra-angle with HXSS connection or torque wrench with surgical driver handle

### Implant Driver TempBase O-Ring (spare part)

EPDM<sup>3</sup>, non-sterile

The Implant Driver TempBase O-Ring is used as spare part for Implant Driver TempBase.

- Multiple use

### Implant Driver EV

Stainless steel<sup>1</sup>, PEEK<sup>4</sup>, non-sterile

The Implant Driver EV is used for installing the implant without using the TempBase EV.

- Multiple use
- Depth marked
- Color coded
- Instruments needed: contra-angle with HXSS connection or torque wrench with surgical driver handle

**The Implant Driver EV is not the standard driver for OmniTaper implants.**


## Planning aids

### OmniTaper Direction Indicator

Titanium<sup>2</sup>, non-sterile

The OmniTaper Direction Indicator is used for visualizing the position and direction of the prepared osteotomy and for measuring the space between osteotomies.

- Multiple use

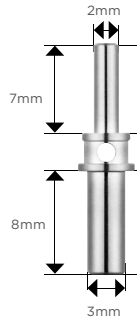

### OmniTaper Direction Indicator




Order No.	68015097
-----------	----------

### OmniTaper Try-In Implants

Titanium alloy<sup>2</sup>, non-sterile

The OmniTaper Direction Indicator is used for intra-operative check of implant position, implant axis, congruency between implant and bone crest, and peri-implant soft tissue level.

- Design matches the DS OmniTaper implant
- Measure the thickness of the soft tissue
- Applicable for all implant lengths
- Multiple use
- Color coded



### OmniTaper Try-In Implants



Ø mm	3.0	3.4	3.8	4.5	5.5
Color coding					
Order No.	68015237	68015238	68015239	68015240	68015241

### Instrument Extender

Stainless steel<sup>3</sup>, non-sterile

The Instrument Extender is used for extending the length of a drill, a tap or the Implant Driver.

- Multiple use

### Instrument Extender



Order No.	68015197
-----------	----------

### OmniTaper Depth Gauge

Titanium alloy<sup>2</sup>, non-sterile

The OmniTaper Depth Gauge is used for measuring the implant site before implant installation.


- Multiple use
- One end corresponds to the implant lengths
- One end is a measuring probe with 0-15 mm markings

### OmniTaper Depth Gauge



Order No.	68015356
-----------	----------

### OmniTaper Radiographic Template

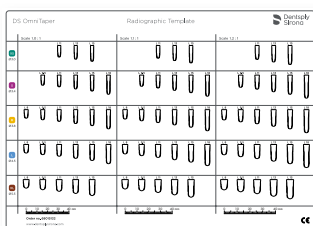

Order No. 68015132

### OmniTaper Radiographic Template

PC<sup>®</sup>, non-sterile

The OmniTaper Radiographic Template is a planning tool used prior to implant surgery.

- Used together with the X-ray of the patient's jaw
- Magnification range from 1.0 to 1.5 presented in two separate sheets

### Torque Wrench EV



Order No. 25774

### Torque Wrench

#### Torque Wrench EV

Stainless steel<sup>1</sup>, non-sterile

The Torque Wrench is used together with the Surgical Driver Handle or the Restorative Driver Handle for tightening and measuring the torque.

- Used together with the Surgical Driver Handle for implant installation and adjustment
- Used together with the Restorative Driver Handle for tightening abutments and/or bridge screws
- Multiple use

### Torque Wrench EV Surgical Driver Handle



Order No. 25775

### Torque Wrench EV Surgical Driver Handle

Stainless steel<sup>1</sup>, non-sterile

The Surgical Driver Handle is used together with the Torque Wrench.

- Multiple use

### Torque Wrench EV Restorative Driver Handle



Order No. 25776 25777

### Torque Wrench EV Restorative Driver Handle

Stainless steel<sup>1</sup>, non-sterile

The Restorative Driver Handle is used together with the Torque Wrench.

- Multiple use

### Hex Driver manual

Stainless steel<sup>1</sup>, non-sterile

The Hex Driver manual is used for tightening screws, and surgical and restorative components.

### Hex Driver manual



Total length mm	20	31
Order No.	25771	25772

### Hex Driver

Stainless steel<sup>1</sup>, non-sterile

The Hex Driver is used for tightening screws, and surgical and restorative components.

### Hex Driver



Total length mm	20	24	35
Order No.	68015207	68015205	68015206

## Surgical Trays

### OmniTaper Surgical Tray

PPSU<sup>2</sup>, silicone<sup>6</sup> holders, non-sterile

The OmniTaper Surgical Tray is used during surgery and storage of OmniTaper surgical instruments.

- Instruments arranged in order of usage
- Two layers for instruments
- Grommet-less solution for easier cleaning
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains no instruments


Please contact customer service to order OmniTaper Surgical Kit (surgical tray and necessary instruments)

### OmniTaper Surgical Tray




Size mm	Length 138	Width 190	Height 61.5
Order No.	68015282		

Upper tray

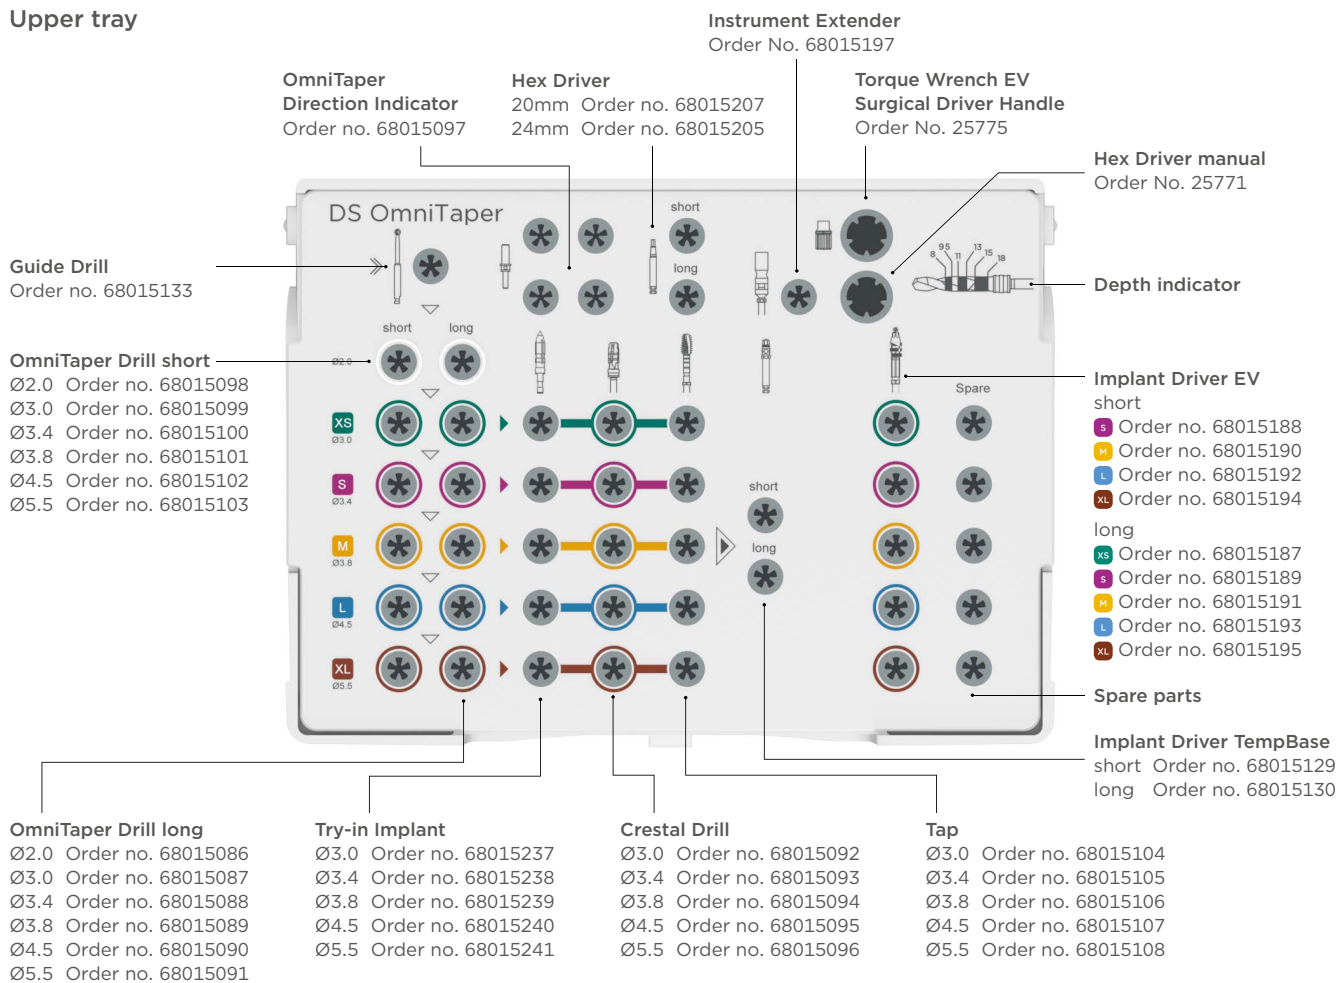

Lower tray

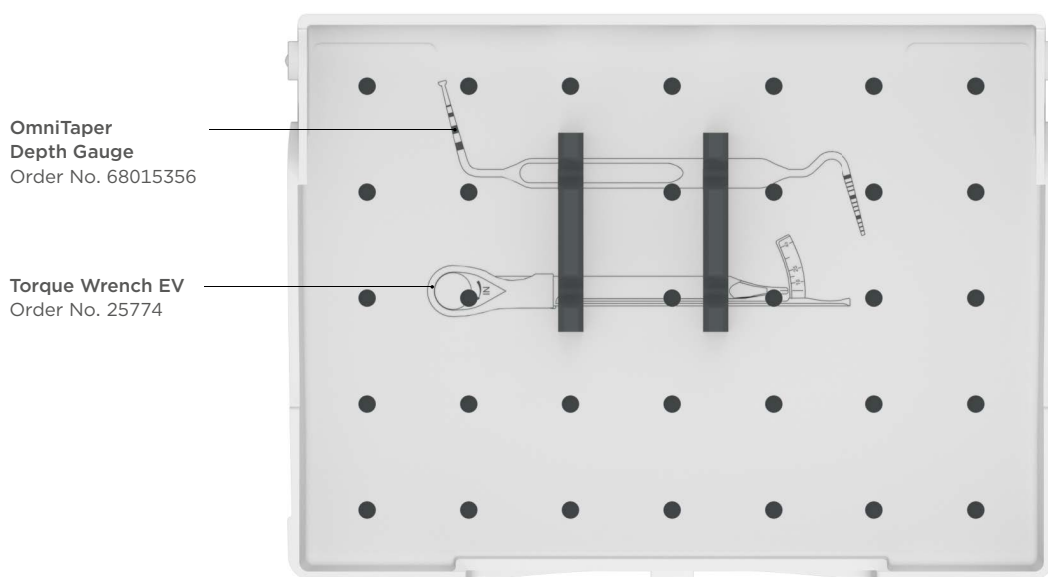

## Washtray & Overlay


### OmniTaper Washtray

Stainless steel<sup>1</sup>, PEEK<sup>6</sup>, silicon<sup>8</sup>, aluminum alloy<sup>5</sup>, non-sterile

The OmniTaper Washtray is used during surgery, for storage, machine cleaning, disinfection and subsequent steam sterilization of OmniTaper surgical instruments.

- Instrument fixation during vertical placement in washer-disinfector
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains: OmniTaper Washtray and removable OmniTaper Washtray Overlay

### OmniTaper Washtray

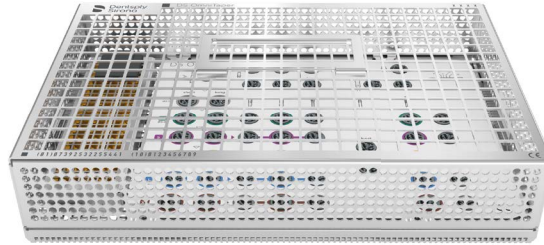

Size mm	Length 276	Width 176	Height 59
Order No.	68015271		

### OmniTaper Washtray Overlay


Aluminum alloy<sup>5</sup>, non-sterile

The OmniTaper Washtray Overlay is used as a spare part for the OmniTaper Washtray.

- Colors and icons supporting surgical procedure

The overlay must be separated from the washtray before cleaning and re-assembled prior to sterilization. For further information, please refer to the Cleaning and sterilization instruction manual.

### OmniTaper Washtray Overlay

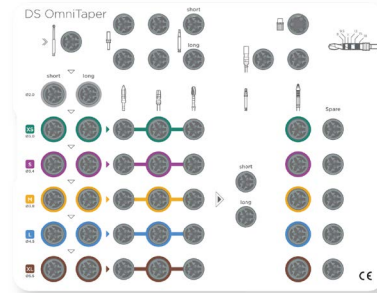

Order No.	68015272
-----------	----------



## Sterilization Container & Reusable Filter

### Washtray Sterilization Container

Aluminum alloy<sup>1</sup>, Stainless steel<sup>1</sup>, PEEK<sup>2</sup>, Silicone<sup>3</sup>, non-sterile

The Washtray Sterilization container is used for sterilization and storage of washtrays.


**The filter needs to be purchased separately**

### Washtray Sterilization Container



Order No.	68015266
-----------	----------

### Reusable Filter for Washtray Sterilization Container

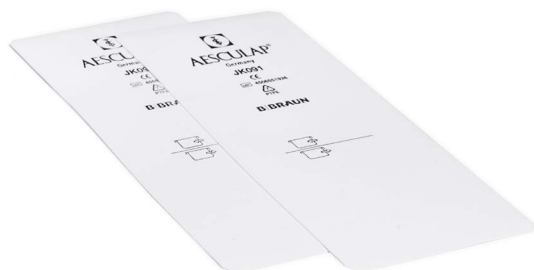

Order No.	68015267
-----------	----------

### Reusable Filter for Washtray Sterilization Container

PTFE<sup>4</sup>, non-sterile

The Reusable Filter for Washtray Sterilization container is used as a spare part for Washtray Sterilization container.

- Multiple use
- Contains: 2 Reusable Filters for Washtray Sterilization Container

# 7. Guided Surgery Instruments

Specific instruments are available for guided implant installation of DS OmniTaper implants. These are marked "GS" (Guided Surgery) and can only be used together with the Simplant SAFE Guide and CEREC Guide 3. When using Simplant software or Simplant planning service, case-specific guided surgery instruments can be ordered with the Simplant SAFE Guide.

## Punch

### OmniTaper Mucosal Punch GS

Stainless steel<sup>1</sup>, sterile

The OmniTaper Mucosal Punch GS is used for minimally-invasive exposure of the surgical site.

- Single use
- Marked with diameter
- Color coded

### OmniTaper Mucosal Punch GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017018	68017019	68017020	68017021

## Drills

### OmniTaper Initial Drill GS

Stainless steel<sup>1</sup>, sterile

The OmniTaper Initial Drill GS is used for creating a starting point for the following drills and removal of soft tissue residue after use of the mucosa punch during guided surgery.

- Multiple use
- Marked with diameter
- Color coded

### OmniTaper Initial Drill GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017111	68017119	68017127	68017135

### OmniTaper Drill GS

Stainless steel<sup>1</sup>, sterile

The OmniTaper Drill GS is used for implant site preparation up to the planned implant diameter.

- Multiple use
- Guided with the sleeve-on-drill system
- Marked with diameter
- Color coded

### OmniTaper Drill GS




Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	8	8	8	8	8
Order No.	68017106	68017114	68017122	68017130	68017137

Drill Sleeve is needed and must be ordered separately

Drills, Crestal drill and Tap for guided surgery can only be used with the contra-angle handpiece.

OmniTaper Drill GS

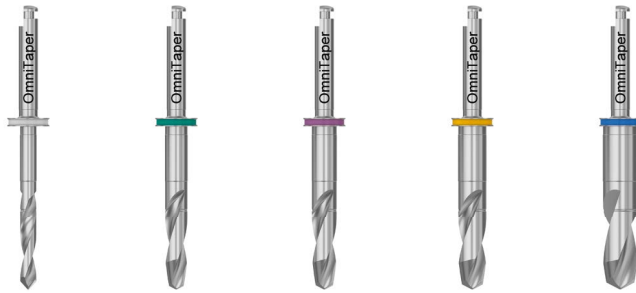

Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	9.5	9.5	9.5	9.5	9.5
Order No.	68017110	68017118	68017126	68017134	68017141



Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	11	11	11	11	11
Order No.	68017107	68017115	68017123	68017131	68017138



Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	13	13	13	13	13
Order No.	68017108	68017116	68017124	68017132	68017139

### OmniTaper Drill GS




Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	15	15	15	15	15
Order No.	68017109	68017117	68017125	68017133	68017140

### OmniTaper Crestal Drill GS

Stainless steel<sup>1</sup>, sterile

The OmniTaper Crestal Drill GS is used for crestal implant site preparation according to the bone quality once the planned implant diameter has been reached.

- Multiple use
- Marked with diameter
- Depth marked
- Color coded



### OmniTaper Crestal Drill GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017100	68017101	68017102	68017103


## Taps

### OmniTaper Tap GS

Stainless steel<sup>1</sup>, sterile

The OmniTaper Tap GS is used for pre-tapping of the implant threads in cortical bone (D I).

- Multiple use
- Marked with diameter
- Depth marked (no mechanical depth stop)
- Color coded



### OmniTaper Tap GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017014	68017015	68017016	68017017

### OmniTaper Drill Sleeve GS narrow diameter



Ø mm	2.0	3.0	3.4	3.8
Order No.	68017105	68017113	68017121	68017129

### OmniTaper Drill Sleeve GS wide diameter



Ø mm	2.0	3.0	3.4	3.8	4.5
Order No.	68017104	68017112	68017120	68017128	68017136

### OmniTaper Implant Driver TempBase GS short



short	ND	WD
Order No.	68017034	68017035

### OmniTaper Implant Driver TempBase GS long



long	ND	WD
Order No.	68017036	68017037

### OmniTaper Sleeve for Implant Driver TempBase GS



Ø	ND	WD
Order No.	68017039	68017038

## Sleeves

### OmniTaper Drill Sleeve GS

Stainless steel<sup>†</sup>, sterile

OmniTaper Drill Sleeve GS is used for safe guidance of the drills in the surgical guide.

- Single use
- Marked with ND (Narrow Diameter) for Ø3.0 - Ø3.8 implants or WD (Wide Diameter) for Ø4.5 implants

**Must be used with the OmniTaper Drill GS**

## Driver

### OmniTaper Implant Driver TempBase GS

Stainless steel<sup>†</sup>, non-sterile

The OmniTaper Driver TempBase GS is used for installing OmniTaper implants with the TempBase using a contra-angle handpiece or the Torque Wrench.

- Markings on the shaft to align the abutment position and to monitor the rotational speed
- Marked with ND (Narrow Diameter) for implant Ø3.0 - Ø3.8 implants
- Marked with WD (Wide Diameter) for implant Ø4.5mm
- Sleeve is pre-mounted and can be replaced
- Torque: ≤ 50 Ncm
- Multiple use

## Sleeves for Driver

### OmniTaper Sleeve for Implant Driver TempBase GS

Stainless steel<sup>†</sup>, non-sterile

The OmniTaper Sleeve for Implant Driver TempBase GS is used as a spare part for the OmniTaper Implant Driver TempBase.

- Multiple use
- Marked with ND (Narrow Diameter) or WD (Wide Diameter)

## Stabilization Abutment

### OmniTaper Stabilization Abutment GS

Titanium alloy<sup>2</sup>, non-sterile

The stabilization abutment GS for TempBase prevents lateral movement of the surgical guide between the preparation of different implant sites and the second stabilization abutment GS. It also prevents the distortion of the guide.

- Multiple use
- Narrow diameter (ND) for Ø3.0 – Ø3.8 implants
- Wide diameter (WD) for Ø4.5 implants

### OmniTaper Stabilization Abutment GS



Ø	ND	WD
Order No.	68017043	68017045

## Positioning Aid

### OmniTaper Positioning Aid EV GS

Titanium alloy<sup>2</sup>, non-sterile

The OmniTaper Positioning Aid EV GS is used to secure implant analogs in the surgical guide in order to transfer the implant position, planned virtually, to a laboratory model (e.g. master cast, plaster cast).

- Multiple use

### OmniTaper Positioning Aid EV GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017040	68017041	68017042	68017044

## Surgical Trays

### OmniTaper Surgical Tray GS

PPSU<sup>2</sup>, silicone<sup>6</sup> holders, non-sterile

The OmniTaper Surgical Tray GS is used during surgery and storage of OmniTaper surgical instruments.

- Two layers for instruments
- Grommet-less solution for easier cleaning
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains no instruments

Please contact customer service to order OmniTaper Surgical Kit GS (surgical tray and necessary instruments)

### OmniTaper Surgical Tray GS



Size mm	Length 138	Width 190	Height 61.5
Order No.	68017203		

**Upper tray**

**OmniTaper Drill GS**

Ø2.0 x 8mm	Order no. 68017106	Ø3.0 x 8mm	Order no. 68017114	Ø3.4 x 8mm	Order no. 68017122	Ø3.8 x 8mm	Order no. 68017130
Ø2.0 x 9.5mm	Order no. 68017110	Ø3.0 x 9.5mm	Order no. 68017118	Ø3.4 x 9.5mm	Order no. 68017126	Ø3.8 x 9.5mm	Order no. 68017134
Ø2.0 x 11mm	Order no. 68017107	Ø3.0 x 11mm	Order no. 68017115	Ø3.4 x 11mm	Order no. 68017123	Ø3.8 x 11mm	Order no. 68017131
Ø2.0 x 13mm	Order no. 68017108	Ø3.0 x 13mm	Order no. 68017116	Ø3.4 x 13mm	Order no. 68017124	Ø3.8 x 13mm	Order no. 68017132
Ø2.0 x 15mm	Order no. 68017109	Ø3.0 x 15mm	Order no. 68017117	Ø3.4 x 15mm	Order no. 68017125	Ø3.8 x 15mm	Order no. 68017133


**OmniTaper Initial Drill GS**

Ø3.0	Order no. 68017111
Ø3.4	Order no. 68017119
Ø3.8	Order no. 68017127
Ø4.5	Order no. 68017135

**OmniTaper Mucosal Punch GS**

Ø3.0	Order no. 68017018
Ø3.4	Order no. 68017019
Ø3.8	Order no. 68017020
Ø4.5	Order no. 68017021

**Torque Wrench EV Surgical Driver Handle**  
Order no. 25775

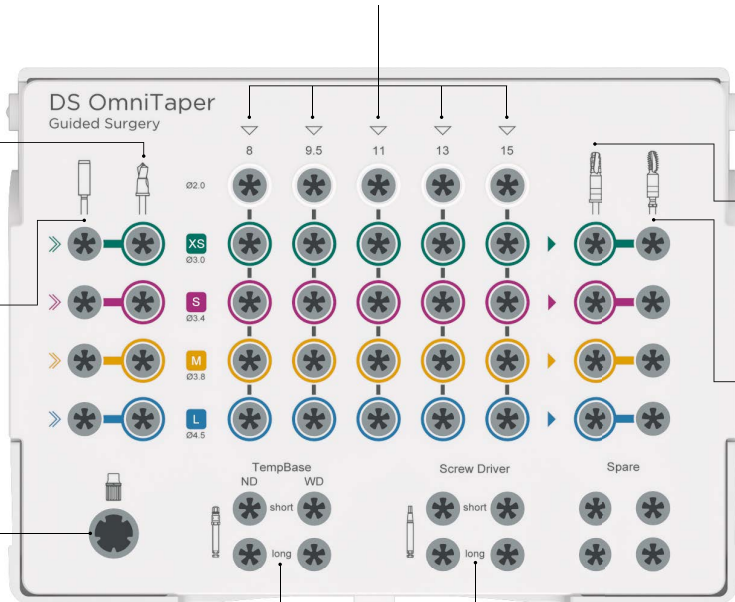

Ø4.5 x 8mm	Order no. 68017137
Ø4.5 x 9.5mm	Order no. 68017141
Ø4.5 x 11mm	Order no. 68017138
Ø4.5 x 13mm	Order no. 68017139
Ø4.5 x 15mm	Order no. 68017140

**OmniTaper Crestal Drill GS**

Ø3.0	Order no. 68017100
Ø3.4	Order no. 68017101
Ø3.8	Order no. 68017102
Ø4.5	Order no. 68017103

**OmniTaper Tap GS**

Ø3.0	Order no. 68017014
Ø3.4	Order no. 68017015
Ø3.8	Order no. 68017016
Ø4.5	Order no. 68017017

**OmniTaper Implant Driver TempBase GS**

ND short	Order no. 68017034
WD short	Order no. 68017035
ND long	Order no. 68017036
WD long	Order no. 68017037

**Hex Driver**


20mm	Order no. 68015207
24mm	Order no. 68015205

**Lower tray**

**OmniTaper Depth Gauge**

Order No. 68015356

**Torque Wrench EV**  
Order No. 25774

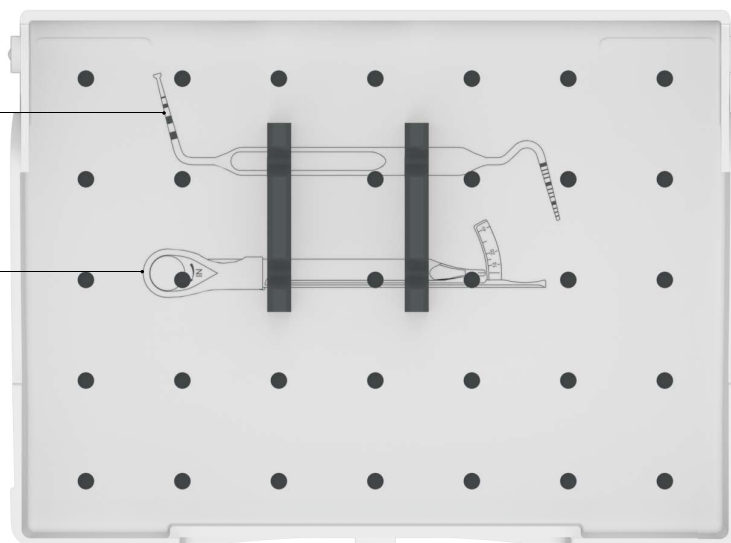


### OmniTaper Washtray GS

Stainless steel<sup>1</sup>, PEEK<sup>2</sup>, silicon<sup>3</sup>, aluminum alloy<sup>2</sup>, non-sterile

The OmniTaper Washtray GS is used during surgery and for storage, machine cleaning, disinfection and subsequent steam sterilization of OmniTaper surgical instruments.

- Instrument fixation during vertical placement in washer-disinfector
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains: OmniTaper Washtray GS and removable OmniTaper Washtray GS Overlay

### OmniTaper Washtray GS

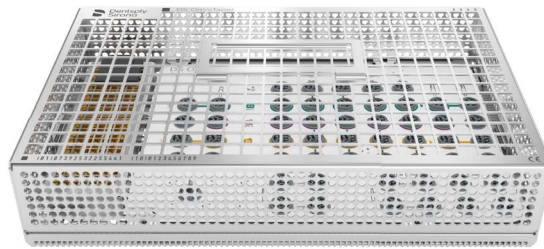

Size mm	Length 276	Width 176	Height 59
Order No.	68015354		

### OmniTaper Washtray GS Overlay


Aluminum alloy<sup>2</sup>, non-sterile

The OmniTaper Washtray GS Overlay is used as a spare part for the OmniTaper Washtray GS.

- Colors and icons supporting surgical procedure

The overlay must be separated from the washtray before cleaning and re-assembled prior to sterilization. For further information, please refer to the Cleaning and sterilization instruction manual.

### OmniTaper Washtray GS Overlay

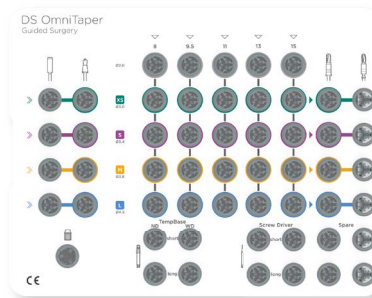

Order No.	68015355
-----------	----------



## 8. Material specifications

Index \* will be found at material description for specific products.

### Metals

Type	Index	Composition/Designation	Standard
Titanium	1	Ti grade 4	ASTM F67
Titanium alloy	2	Ti6Al4V ELI	ASTM F136
Stainless steel	3	Surgical stainless steel	ASTM F899
TiN Coating	4	Titanium Nitride	
Aluminum alloy	5	AlMg1	
Titanium	12	Ti grade 2	ASTM F67

### Plastics

Type	Index	Composition/Designation	Standard
PEEK	6	Polyetheretherketone	
PPSU	7	Polyphenylsulfone	
Silicone	8	Polysiloxane	
ABS	9	Acrylonitrile butadiene styrene	
PC	10	Polycarbonate	
PP	11	Polypropylene	
EPDM	13	Ethylene propylene diene rubber	
PTFE	14	Polytetrafluoroethylene	

# 9. Index

## By order number

Order No.		page
25771	Hex Driver 20mm manual.....	14
25772	Hex Driver 31mm manual.....	14
25774	Torque Wrench EV.....	13
25775	Torque Wrench EV Surgical Driver Handle.....	13
25776	Torque Wrench EV Rest. Driver Handle.....	13
25777	Torque Wrench EV Rest. Driver Handle Low.....	13
68010001	Cover Screw EV (XS).....	6
68010002	Cover Screw EV (S).....	6
68010005	Cover Screw EV (M).....	6
68010006	Cover Screw EV (L).....	6
68010007	Cover Screw EV (XL).....	6
68010013	TempBase Cap (XS)-(M).....	6
68010014	TempBase Cap (L).....	6
68010015	TempBase Cap (XL).....	6
68011140	OmniTaper EV Ø3.0 x 11mm.....	5
68011141	OmniTaper EV Ø3.0 x 13mm.....	5
68011142	OmniTaper EV Ø3.0 x 15mm.....	5
68011143	OmniTaper EV Ø3.4 x 9.5mm.....	5
68011144	OmniTaper EV Ø3.4 x 11mm.....	5
68011145	OmniTaper EV Ø3.4 x 13mm.....	5
68011146	OmniTaper EV Ø3.4 x 15mm.....	5
68011147	OmniTaper EV Ø3.4 x 18mm.....	5
68011148	OmniTaper EV Ø3.8 x 8mm.....	5
68011149	OmniTaper EV Ø3.8 x 9.5mm.....	5
68011150	OmniTaper EV Ø3.8 x 11mm.....	5
68011151	OmniTaper EV Ø3.8 x 13mm.....	5
68011152	OmniTaper EV Ø3.8 x 15mm.....	5
68011153	OmniTaper EV Ø3.8 x 18mm.....	5
68011154	OmniTaper EV Ø4.5 x 8mm.....	5
68011155	OmniTaper EV Ø4.5 x 9.5mm.....	5
68011156	OmniTaper EV Ø4.5 x 11mm.....	5
68011157	OmniTaper EV Ø4.5 x 13mm.....	5
68011158	OmniTaper EV Ø4.5 x 15mm.....	5
68011159	OmniTaper EV Ø4.5 x 18mm.....	5
68011160	OmniTaper EV Ø5.5 x 8mm.....	5
68011161	OmniTaper EV Ø5.5 x 9.5mm.....	5
68011162	OmniTaper EV Ø5.5 x 11mm.....	5
68011163	OmniTaper EV Ø5.5 x 13mm.....	5
68011164	OmniTaper EV Ø5.5 x 15mm.....	5
68013001	HealDesign EV (XS) Ø3.5 2.5mm.....	6
68013002	HealDesign EV (XS) Ø3.5 3.5mm.....	6
68013003	HealDesign EV (XS) Ø3.5 4.5mm.....	6
68013004	HealDesign EV (XS) Ø3.5 6.5mm.....	6
68013005	HealDesign EV (S) Ø4.0 2.5mm.....	7
68013006	HealDesign EV (S) Ø4.0 3.5mm.....	7
68013007	HealDesign EV (S) Ø4.0 4.5mm.....	7
68013008	HealDesign EV (S) Ø4.0 6.5mm.....	7
68013009	HealDesign EV (S) Ø5.0 2.5mm.....	7
68013010	HealDesign EV (S) Ø5.0 3.5mm.....	7
68013011	HealDesign EV (S) Ø5.0 4.5mm.....	7
68013012	HealDesign EV (S) Ø5.0 6.5mm.....	7
68013013	HealDesign EV (S) Ø6.0 3.5mm.....	7
68013014	HealDesign EV (S) Ø6.0 4.5mm.....	7
68013015	HealDesign EV (M) Ø5.0 2.5mm.....	7
68013016	HealDesign EV (M) Ø5.0 3.5mm.....	7
68013017	HealDesign EV (M) Ø5.0 4.5mm.....	7
68013018	HealDesign EV (M) Ø5.0 6.5mm.....	7
68013019	HealDesign EV (M) Ø6.5 2.5mm.....	7
68013020	HealDesign EV (M) Ø6.5 3.5mm.....	7
68013021	HealDesign EV (M) Ø6.5 4.5mm.....	7
68013022	HealDesign EV (M) Ø6.5 6.5mm.....	7
68013023	HealDesign EV (L) Ø5.0 2.5mm.....	7
68013024	HealDesign EV (L) Ø5.0 3.5mm.....	7
68013025	HealDesign EV (L) Ø5.0 4.5mm.....	7
68013026	HealDesign EV (L) Ø5.0 6.5mm.....	7

Order No.		page
68013027	HealDesign EV (L) Ø6.5 2.5mm.....	7
68013028	HealDesign EV (L) Ø6.5 3.5mm.....	7
68013029	HealDesign EV (L) Ø6.5 4.5mm.....	7
68013030	HealDesign EV (L) Ø6.5 6.5mm.....	7
68013031	HealDesign EV (L) Ø7.5 3.5mm.....	7
68013032	HealDesign EV (L) Ø7.5 4.5mm.....	7
68013033	HealDesign EV (XL) Ø6.5 2.5mm.....	7
68013034	HealDesign EV (XL) Ø6.5 3.5mm.....	7
68013035	HealDesign EV (XL) Ø6.5 4.5mm.....	7
68013036	HealDesign EV (XL) Ø6.5 6.5mm.....	7
68013037	HealDesign EV (XL) Ø7.5 3.5mm.....	7
68013038	HealDesign EV (XL) Ø7.5 4.5mm.....	7
68013039	HealDesign EV (S) Ø5.0 3.5mm Triangular.....	7
68013040	HealDesign EV (M) Ø5.0 3.5mm Triangular.....	7
68013041	HealDesign EV (M) Ø6.5 3.5mm Triangular.....	7
68013042	HealDesign EV (L) Ø5.0 3.5mm Triangular.....	7
68013043	HealDesign EV (L) Ø6.5 3.5mm Triangular.....	7
68013044	Healing Abutment EV (XS) 2mm.....	8
68013045	Healing Abutment EV (XS) 3mm.....	8
68013046	Healing Abutment EV (XS) 4mm.....	8
68013047	Healing Abutment EV (XS) 6mm.....	8
68013048	Healing Abutment EV (S) 2mm.....	8
68013049	Healing Abutment EV (S) 3mm.....	8
68013050	Healing Abutment EV (S) 4mm.....	8
68013051	Healing Abutment EV (S) 6mm.....	8
68013052	Healing Abutment EV (M) 2mm.....	8
68013053	Healing Abutment EV (M) 3mm.....	8
68013054	Healing Abutment EV (M) 4mm.....	8
68013055	Healing Abutment EV (M) 6mm.....	8
68013056	Healing Abutment EV (L) 2mm.....	8
68013057	Healing Abutment EV (L) 3mm.....	8
68013058	Healing Abutment EV (L) 4mm.....	8
68013059	Healing Abutment EV (L) 6mm.....	8
68013060	Healing Abutment EV (XL) 2mm.....	8
68013061	Healing Abutment EV (XL) 3mm.....	8
68013062	Healing Abutment EV (XL) 4mm.....	8
68013063	Healing Abutment EV (XL) 6mm.....	8
68015080	OmniTaper Drill SP Ø2.0 short.....	10
68015081	OmniTaper Drill SP Ø3.0 short.....	10
68015082	OmniTaper Drill SP Ø3.4 short.....	10
68015083	OmniTaper Drill SP Ø3.8 short.....	10
68015084	OmniTaper Drill SP Ø4.5 short.....	10
68015085	OmniTaper Drill SP Ø5.5 short.....	10
68015086	OmniTaper Drill Ø2.0 long.....	9
68015087	OmniTaper Drill Ø3.0 long.....	9
68015088	OmniTaper Drill Ø3.4 long.....	9
68015089	OmniTaper Drill Ø3.8 long.....	9
68015090	OmniTaper Drill Ø4.5 long.....	9
68015091	OmniTaper Drill Ø5.5 long.....	9
68015092	OmniTaper Crestal Drill Ø3.0.....	10
68015093	OmniTaper Crestal Drill Ø3.4.....	10
68015094	OmniTaper Crestal Drill Ø3.8.....	10
68015095	OmniTaper Crestal Drill Ø4.5.....	10
68015096	OmniTaper Crestal Drill Ø5.5.....	10
68015097	OmniTaper Direction Indicator.....	12
68015098	OmniTaper Drill Ø2.0 short.....	9
68015099	OmniTaper Drill Ø3.0 short.....	9
68015100	OmniTaper Drill Ø3.4 short.....	9
68015101	OmniTaper Drill Ø3.8 short.....	9
68015102	OmniTaper Drill Ø4.5 short.....	9
68015103	OmniTaper Drill Ø5.5 short.....	9
68015104	OmniTaper Tap Ø3.0.....	10
68015105	OmniTaper Tap Ø3.4.....	10
68015106	OmniTaper Tap Ø3.8.....	10
68015107	OmniTaper Tap Ø4.5.....	10

Order No.	page	Order No.	page
68015108	10	68017041	22
68015129	11	68017042	22
68015130	11	68017043	22
68015131	11	68017044	22
68015132	13	68017045	22
68015133	9	68017100	20
68015134	9	68017101	20
68015187	11	68017102	20
68015188	11	68017103	20
68015189	11	68017104	21
68015190	11	68017105	21
68015191	11	68017106	18
68015192	11	68017107	19
68015193	11	68017108	19
68015194	11	68017109	20
68015195	11	68017110	19
68015197	12	68017111	18
68015205	14	68017112	21
68015206	14	68017113	21
68015207	14	68017114	18
68015237	12	68017115	19
68015238	12	68017116	19
68015239	12	68017117	20
68015240	12	68017118	19
68015241	12	68017119	18
68015266	17	68017120	21
68015267	17	68017121	21
68015271	16	68017122	18
68015272	16	68017123	19
68015282	14	68017124	19
68015354	24	68017125	20
68015355	24	68017126	19
68015356	12	68017127	18
68017014	20	68017128	21
68017015	20	68017129	21
68017016	20	68017130	18
68017017	20	68017131	19
68017018	18	68017132	19
68017019	18	68017133	20
68017020	18	68017134	19
68017021	18	68017135	18
68017034	21	68017136	21
68017035	21	68017137	18
68017036	21	68017138	19
68017037	21	68017139	19
68017038	21	68017140	20
68017039	21	68017141	19
68017040	22	68017203	22

## Alphabetical order

Order No.		page	Order No.		page
68010006	Cover Screw EV (L).....	6	68013044	Healing Abutment EV (XS) 2mm.....	8
68010005	Cover Screw EV (M).....	6	68013045	Healing Abutment EV (XS) 3mm.....	8
68010002	Cover Screw EV (S).....	6	68013046	Healing Abutment EV (XS) 4mm.....	8
68010007	Cover Screw EV (XL).....	6	68013047	Healing Abutment EV (XS) 6mm.....	8
68010001	Cover Screw EV (XS).....	6	68015207	Hex Driver 20mm.....	14
68015133	Guide Drill.....	9	25771	Hex Driver 20mm manual.....	14
68013023	HealDesign EV (L) Ø5.0 2.5mm.....	7	68015205	Hex Driver 24mm.....	14
68013024	HealDesign EV (L) Ø5.0 3.5mm.....	7	25772	Hex Driver 31mm manual.....	14
68013042	HealDesign EV (L) Ø5.0 3.5mm Triangular.....	7	68015206	Hex Driver 35mm.....	14
68013025	HealDesign EV (L) Ø5.0 4.5mm.....	7	68015193	Implant Driver EV (L) long.....	11
68013026	HealDesign EV (L) Ø5.0 6.5mm.....	7	68015192	Implant Driver EV (L) short.....	11
68013027	HealDesign EV (L) Ø6.5 2.5mm.....	7	68015191	Implant Driver EV (M) long.....	11
68013028	HealDesign EV (L) Ø7.5 3.5mm.....	7	68015190	Implant Driver EV (M) short.....	11
68013043	HealDesign EV (L) Ø6.5 3.5mm Triangular.....	7	68015189	Implant Driver EV (S) long.....	11
68013029	HealDesign EV (L) Ø6.5 4.5mm.....	7	68015188	Implant Driver EV (S) short.....	11
68013030	HealDesign EV (L) Ø6.5 6.5mm.....	7	68015195	Implant Driver EV (XL) long.....	11
68013031	HealDesign EV (L) Ø7.5 3.5mm.....	7	68015194	Implant Driver EV (XL) short.....	11
68013032	HealDesign EV (L) Ø7.5 4.5mm.....	7	68015187	Implant Driver EV (XS) long.....	11
68013015	HealDesign EV (M) Ø5.0 2.5mm.....	7	68015130	Implant Driver TempBase long.....	11
68013016	HealDesign EV (M) Ø5.0 3.5mm.....	7	68015131	Implant Driver TempBase O-Ring.....	11
68013040	HealDesign EV (M) Ø5.0 3.5mm Triangular.....	7	68015129	Implant Driver TempBase short.....	11
68013017	HealDesign EV (M) Ø5.0 4.5mm.....	7	68015197	Instrument Extender.....	12
68013018	HealDesign EV (M) Ø5.0 6.5mm.....	7	68015092	OmniTaper Crestal Drill Ø3.0.....	10
68013019	HealDesign EV (M) Ø6.5 2.5mm.....	7	68017100	OmniTaper Crestal Drill Ø3.0 GS.....	20
68013020	HealDesign EV (M) Ø6.5 3.5mm.....	7	68015093	OmniTaper Crestal Drill Ø3.4.....	10
68013041	HealDesign EV (M) Ø6.5 3.5mm Triangular.....	7	68017101	OmniTaper Crestal Drill Ø3.4 GS.....	20
68013021	HealDesign EV (M) Ø6.5 4.5mm.....	7	68015094	OmniTaper Crestal Drill Ø3.8.....	10
68013022	HealDesign EV (M) Ø6.5 6.5mm.....	7	68017102	OmniTaper Crestal Drill Ø3.8 GS.....	20
68013005	HealDesign EV (S) Ø4.0 2.5mm.....	7	68015095	OmniTaper Crestal Drill Ø4.5.....	10
68013006	HealDesign EV (S) Ø4.0 3.5mm.....	7	68017103	OmniTaper Crestal Drill Ø4.5 GS.....	20
68013007	HealDesign EV (S) Ø4.0 4.5mm.....	7	68015096	OmniTaper Crestal Drill Ø5.5.....	10
68013008	HealDesign EV (S) Ø4.0 6.5mm.....	7	68015356	OmniTaper Depth Gauge.....	12
68013009	HealDesign EV (S) Ø5.0 2.5mm.....	7	68015097	OmniTaper Direction Indicator.....	12
68013010	HealDesign EV (S) Ø5.0 3.5mm.....	7	68015086	OmniTaper Drill Ø2.0 long.....	9
68013039	HealDesign EV (S) Ø5.0 3.5mm Triangular.....	7	68015098	OmniTaper Drill Ø2.0 short.....	9
68013011	HealDesign EV (S) Ø5.0 4.5mm.....	7	68017106	OmniTaper Drill Ø2.0 x 8mm GS.....	18
68013012	HealDesign EV (S) Ø5.0 6.5mm.....	7	68017110	OmniTaper Drill Ø2.0 x 9.5mm GS.....	19
68013013	HealDesign EV (S) Ø6.0 3.5mm.....	7	68017107	OmniTaper Drill Ø2.0 x 11mm GS.....	19
68013014	HealDesign EV (S) Ø6.0 4.5mm.....	7	68017108	OmniTaper Drill Ø2.0 x 13mm GS.....	19
68013033	HealDesign EV (XL) Ø6.5 2.5mm.....	7	68017109	OmniTaper Drill Ø2.0 x 15mm GS.....	20
68013034	HealDesign EV (XL) Ø6.5 3.5mm.....	7	68015087	OmniTaper Drill Ø3.0 long.....	9
68013035	HealDesign EV (XL) Ø6.5 4.5mm.....	7	68015099	OmniTaper Drill Ø3.0 short.....	9
68013036	HealDesign EV (XL) Ø6.5 6.5mm.....	7	68017114	OmniTaper Drill Ø3.0 x 8mm GS.....	18
68013037	HealDesign EV (XL) Ø7.5 3.5mm.....	7	68017118	OmniTaper Drill Ø3.0 x 9.5mm GS.....	19
68013038	HealDesign EV (XL) Ø7.5 4.5mm.....	7	68017115	OmniTaper Drill Ø3.0 x 11mm GS.....	19
68013001	HealDesign EV (XS) Ø3.5 2.5mm.....	6	68017116	OmniTaper Drill Ø3.0 x 13mm GS.....	19
68013002	HealDesign EV (XS) Ø3.5 3.5mm.....	6	68017117	OmniTaper Drill Ø3.0 x 15mm GS.....	20
68013003	HealDesign EV (XS) Ø3.5 4.5mm.....	6	68015088	OmniTaper Drill Ø3.4 long.....	9
68013004	HealDesign EV (XS) Ø3.5 6.5mm.....	6	68015100	OmniTaper Drill Ø3.4 short.....	9
68013056	Healing Abutment EV (L) 2mm.....	8	68017122	OmniTaper Drill Ø3.4 x 8mm GS.....	18
68013057	Healing Abutment EV (L) 3mm.....	8	68017126	OmniTaper Drill Ø3.4 x 9.5mm GS.....	19
68013058	Healing Abutment EV (L) 4mm.....	8	68017123	OmniTaper Drill Ø3.4 x 11mm GS.....	19
68013059	Healing Abutment EV (L) 6mm.....	8	68017124	OmniTaper Drill Ø3.4 x 13mm GS.....	19
68013052	Healing Abutment EV (M) 2mm.....	8	68017125	OmniTaper Drill Ø3.4 x 15mm GS.....	20
68013053	Healing Abutment EV (M) 3mm.....	8	68015089	OmniTaper Drill Ø3.8 long.....	9
68013054	Healing Abutment EV (M) 4mm.....	8	68015101	OmniTaper Drill Ø3.8 short.....	9
68013055	Healing Abutment EV (M) 6mm.....	8	68017130	OmniTaper Drill Ø3.8 x 8mm GS.....	18
68013048	Healing Abutment EV (S) 2mm.....	8	68017134	OmniTaper Drill Ø3.8 x 9.5mm GS.....	19
68013049	Healing Abutment EV (S) 3mm.....	8	68017131	OmniTaper Drill Ø3.8 x 11mm GS.....	19
68013050	Healing Abutment EV (S) 4mm.....	8	68017132	OmniTaper Drill Ø3.8 x 13mm GS.....	19
68013051	Healing Abutment EV (S) 6mm.....	8	68017133	OmniTaper Drill Ø3.8 x 15mm GS.....	20
68013060	Healing Abutment EV (XL) 2mm.....	8	68015090	OmniTaper Drill Ø4.5 long.....	9
68013061	Healing Abutment EV (XL) 3mm.....	8	68015102	OmniTaper Drill Ø4.5 short.....	9
68013062	Healing Abutment EV (XL) 4mm.....	8	68017137	OmniTaper Drill Ø4.5 x 8mm GS.....	18
68013063	Healing Abutment EV (XL) 6mm.....	8	68017141	OmniTaper Drill Ø4.5 x 9.5mm GS.....	19

Order No.	page	Order No.	page
68017138	19	68017035	21
68017139	19	68017111	18
68017140	20	68017119	18
68015091	9	68017127	18
68015103	9	68017135	18
68017105	21	68017018	18
68017113	21	68017019	18
68017121	21	68017020	18
68017129	21	68017021	18
68017104	21	68017044	22
68017112	21	68017042	22
68017120	21	68017041	22
68017128	21	68017040	22
68017136	21	68015132	13
68015080	10	68017039	21
68015081	10	68017038	21
68015082	10	68017043	22
68015083	10	68017045	22
68015084	10	68015282	14
68015085	10	68017203	22
68011140	5	68015104	10
68011141	5	68017014	20
68011142	5	68015105	10
68011143	5	68017015	20
68011144	5	68015106	10
68011145	5	68017016	20
68011146	5	68015107	10
68011147	5	68017017	20
68011148	5	68015108	10
68011149	5	68015237	12
68011150	5	68015238	12
68011151	5	68015239	12
68011152	5	68015240	12
68011153	5	68015241	12
68011154	5	68015271	16
68011155	5	68015354	24
68011156	5	68015272	16
68011157	5	68015355	24
68011158	5	68015134	9
68011159	5	68010014	6
68011160	5	68010015	6
68011161	5	68010013	6
68011162	5	25774	13
68011163	5	25776	13
68011164	5	25775	13
68017036	21	25777	13
68017034	21	68015266	17
68017037	21	68015267	17





---

THE DENTAL  
SOLUTIONS  
COMPANY™

